


QBTA: ON [ALT-F1/BB=60]

Pile Dynamics, Inc.

DPF

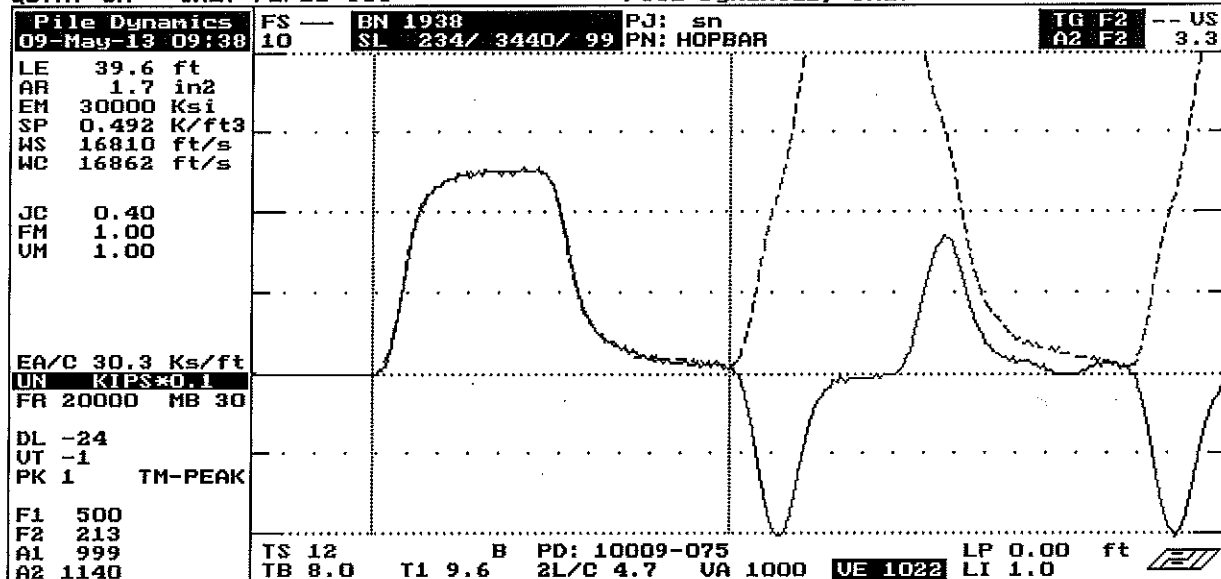

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.1 FMX= 64 AMX= 159
	EMX= 0.3 MEX= 125 FUP= 1.00



contact Pile Dynamics USA
with your questions
tel USA - 216 - 831- 6131
fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION N.I.S.T. Traceable

SERIAL NUMBER: 10009

CALIBRATION FACTOR: 1140 G/v

PAK (*5000) DATE: 09-MAY-13

PDA OPERATOR: *[Signature]*

<-AT:PIEZORESISTIVE

OP: alex [ver:4.05]

[AT:PIEZOELECTRIC->