


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

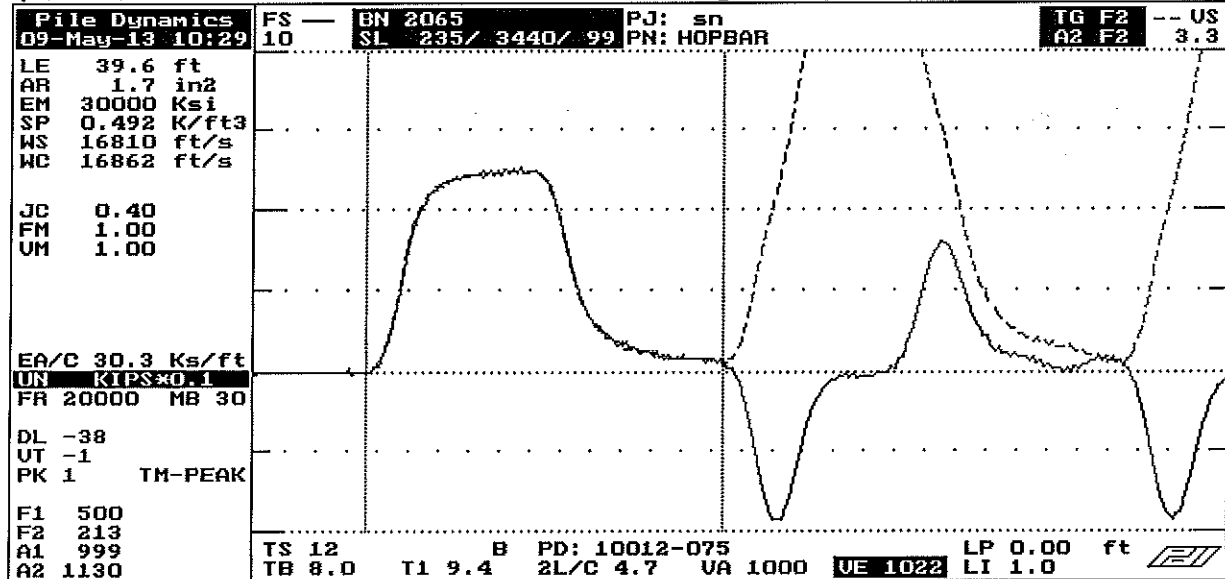

ACCEPT SQ-OFF FL-OFF PR-OFF

VMX= 4.1 FMX= 63 AMX= 149
 EMX= 0.3 MEX= 123 FVP= 1.00



contact File Dynamics USA
 with your questions
 tel USA - 216 - 831- 6131
 fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION N.I.S.T. Traceable

SERIAL NUMBER: 10012

CALIBRATION FACTOR: 1130 G/v

PAK (*5000): DATE: 09-MAY-13

PDA OPERATOR: *[Signature]*

<-AT:PIEZORESISTIVE

OP: alex lver:4.051

AT:PIEZOELECTRIC->