


QBTA: ON [ALT-F1/BB=60]

Pile Dynamics, Inc.

DPF

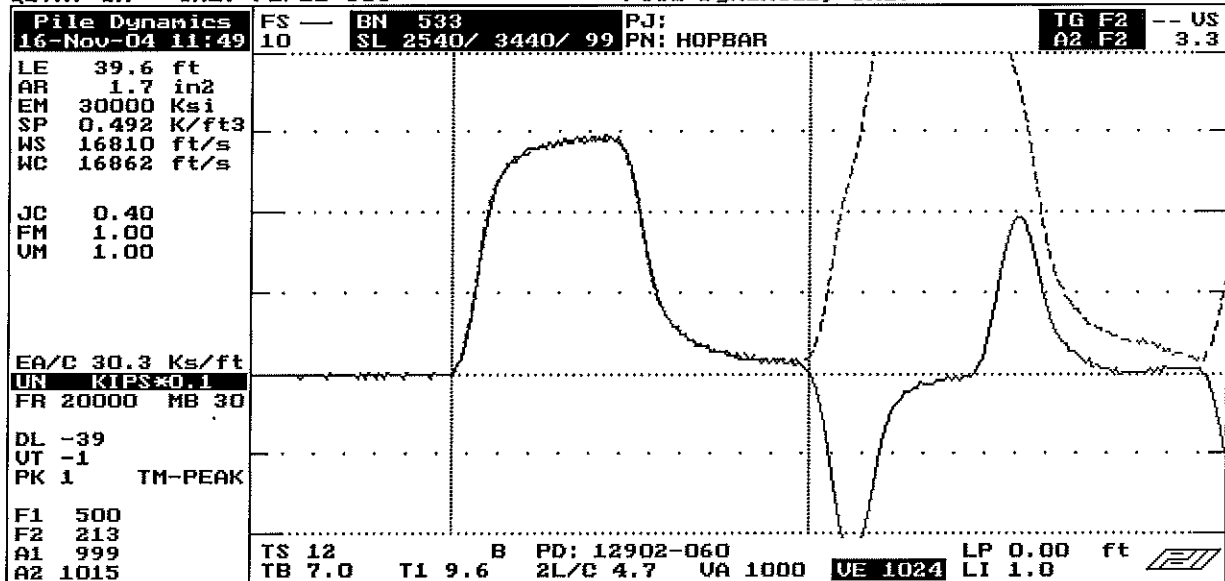

ACCEPT SQ-OFF FL-OFF PR-OFF



contact Pile Dynamics USA
 with your questions
 tel USA - 216 - 831- 6131
 fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION

N.I.S.T. Traceable

SERIAL NUMBER: 12902

CALIBRATION FACTOR: 1015 G/V

PAK (#5000):

DATE: 16-Nov-04

PDA OPERATOR: Fred Hudson

<-AT:PIEZORESISTIVE

OP: FRED Iver:4.05]

[AT:PIEZOELECTRIC->