


QBTA: ON [ALT-F1/BB=601]

Pile Dynamics, Inc.

DPF

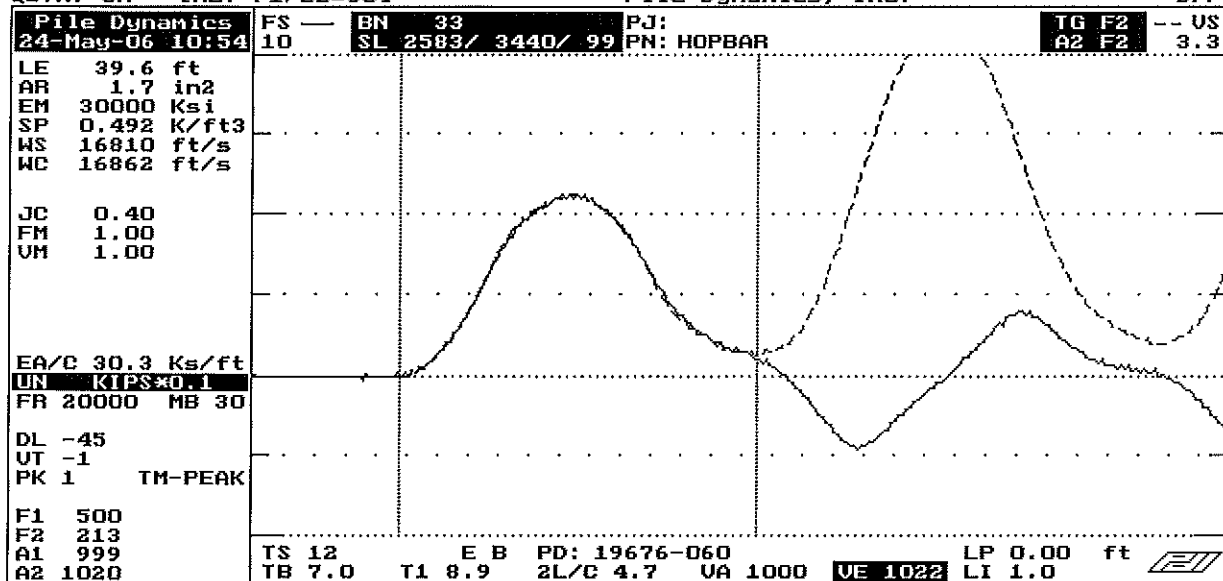

contact Pile Dynamics USA
 with your questions
 tel USA - 216 - 831- 6131
 fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION N.I.S.T. Traceable
 SERIAL NUMBER: 19676
 CALIBRATION FACTOR: 1020 G/V
 PAK (45000): DATE: 24-May-06
 PDA OPERATOR: *David H.*

<-AT:PIEZORESISTIVE

OP: DAVE [ver:4.05]

AT:PIEZOELECTRIC->