


QBTA: ON IALT-F1/BB=601

File Dynamics, Inc.

DPF

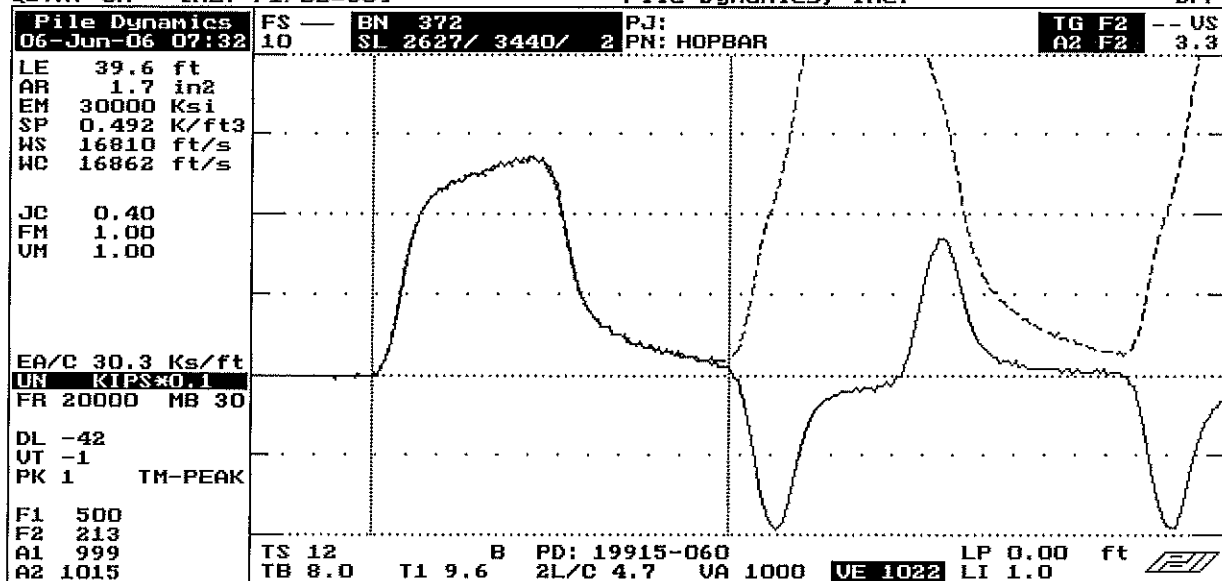

ACCEPT SQ-OFF FL-OFF PR-OFF



contact File Dynamics USA
 with your questions
 tel USA - 216 - 831- 6131
 fax USA - 216 - 831- 0916

VMX= 4.3 FMX= 68 AMX= 159
 EMX= 0.3 MEX= 133 FUP= 1.00

ACCELEROMETER CALIBRATION N.I.S.T. Traceable

SERIAL NUMBER: 19915

CALIBRATION FACTOR: 1015 G/V

PAK (X5000): DATE: 06-JUN-06

PDA OPERATOR: Fred Iver

<-AT:PIEZORESISTIVE

OP: fred Iver:4.051

AT:PIEZOELECTRIC->