


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

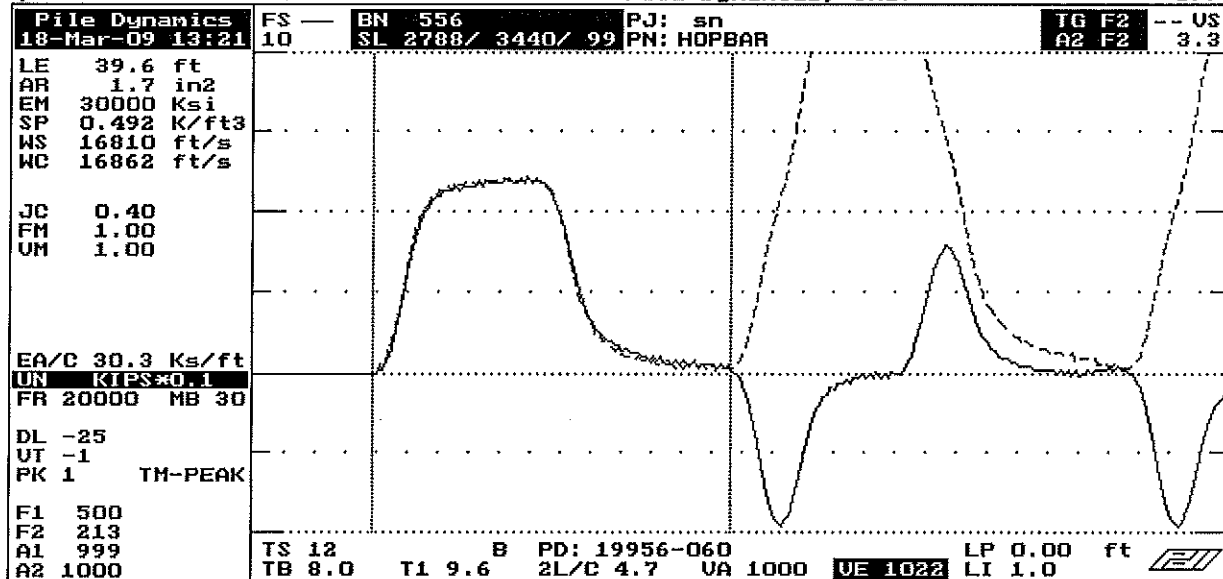

ACCEPT SQ-OFF FL-OFF PR-OFF	VMX= 4.0 FMX= 61 AMX= 149
	EMX= 0.2 MEX= 119 FVP= 0.98
 contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916	ACCELEROMETER CALIBRATION N.I.S.T. Traceable
	SERIAL NUMBER: 19956
	CALIBRATION FACTOR: 1000 g/v
	DATE: 18-MAR-09
PDA OPERATOR: [Signature]	

<-AT:PIEZORESISTIVE

OP: alex [ver:4.05]

[AT:PIEZOELECTRIC->