


QBTA: ON [ALT-F1/BB=60]

Pile Dynamics, Inc.

DPF

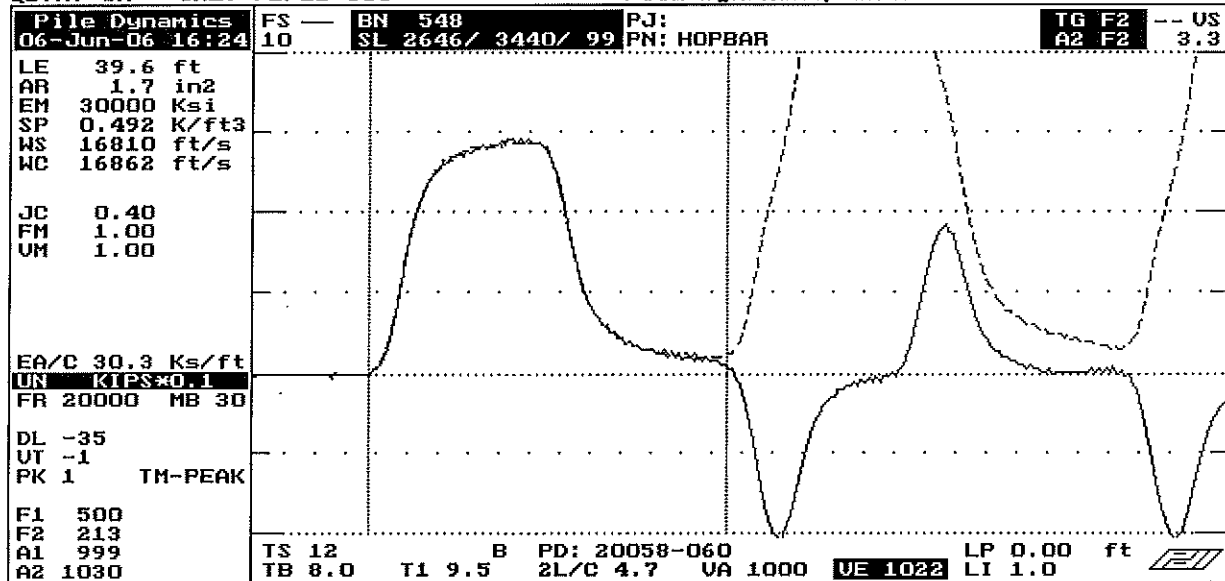

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.7	FMX= 73	AMX= 159
	EMX= 0.3	MEX= 143	FVP= 1.00
 contact Pile Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916	ACCELEROMETER CALIBRATION N.I.S.T. Traceable		
	SERIAL NUMBER: 20058		
	CALIBRATION FACTOR: 1030 G/V		
	PAK (5000): DATE: 06-JUN-06		
PDA OPERATOR: <i>[Signature]</i>			

<-AT:PIEZORESISTIVE

OP: fred Iver:4.051

AT:PIEZOELECTRIC->