


QBTA: ON IALT-F1/BB=601

File Dynamics, Inc.

DPF

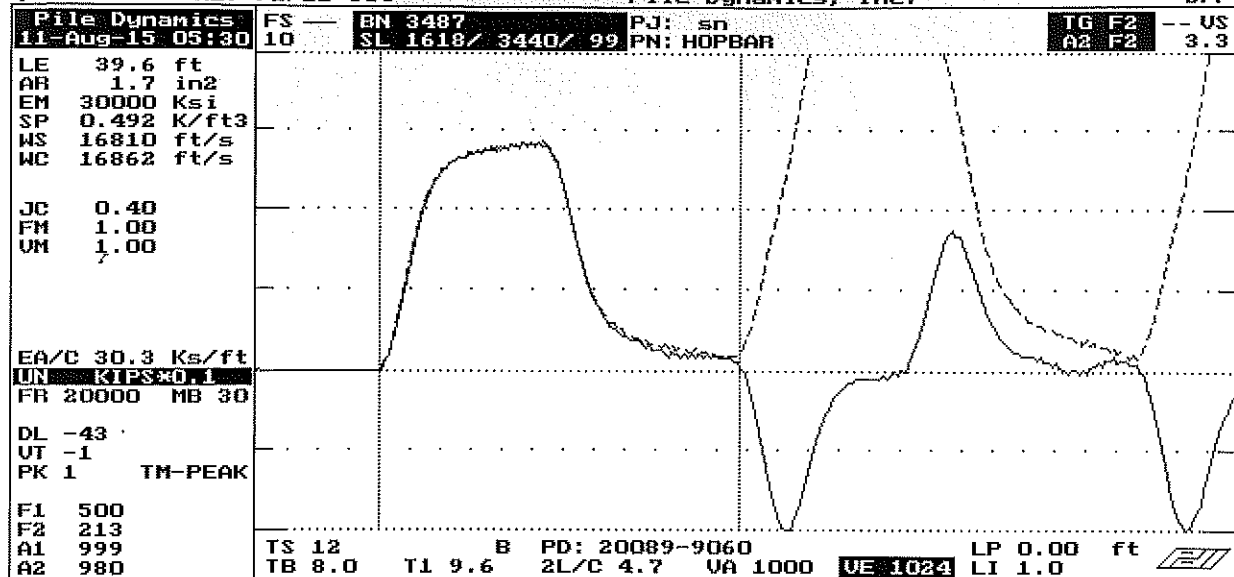

ACCEPT SQ-OFF FL-OFF PR-OFF	VMX= 4.6 FMX= 71 AMX= 149 EMX= 0.3 MEX= 139 FVP= 0.98
contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916	ACCELEROMETER CALIBRATION N.I.S.T. Traceable SERIAL NUMBER: 20089 CALIBRATION FACTOR: 980% PAK (*5000): DATE: 3AUG15 PDA OPERATOR: <i>[Signature]</i> OP: laine lver:4.051
<-AT:PIEZORESISTIVE	AT:PIEZOELECTRIC->