




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: X776  
 PDI Gage Factor: 93.4  
 Mean Linear Correlation Coefficient: 0.999961

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-1916.0	-5.952	481.2	1.553
-1430.4	-4.458	839.9	2.682
-975.5	-3.036	1168.0	3.717
-590.6	-1.828	1509.2	4.766
-282.2	-0.852	1837.3	5.745
45.9	0.193	1996.9	6.226

Calibration Curve

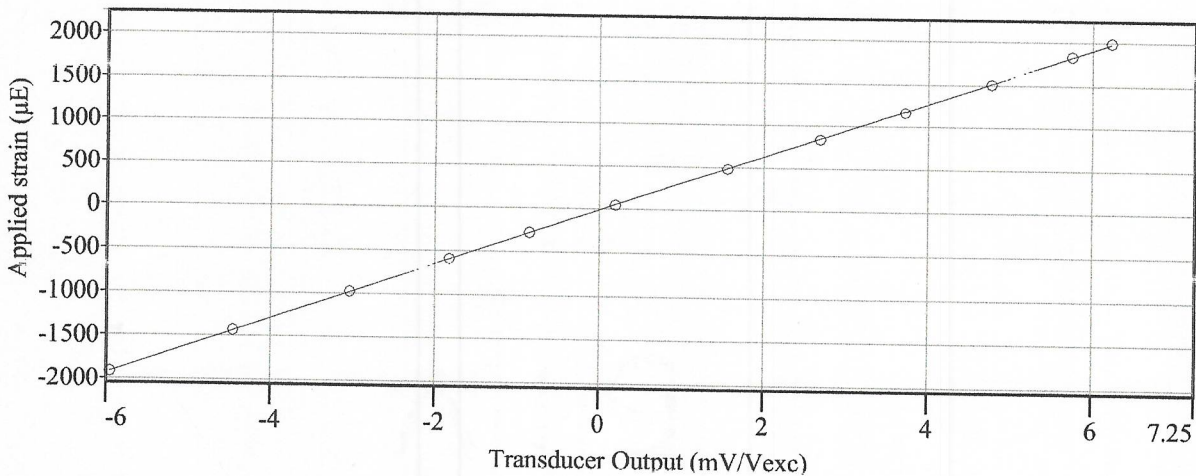

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: X776

Calibration Date: FEB 02 2023

