




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: X779
 PDI Gage Factor: 93.6
 Mean Linear Correlation Coefficient: 0.999950

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1902.9	-5.952	498.7	1.580
-1423.9	-4.450	839.9	2.666
-964.6	-3.023	1161.4	3.661
-597.1	-1.857	1482.9	4.654
-282.2	-0.866	1802.3	5.585
65.6	0.217	2007.9	6.216

Calibration Curve

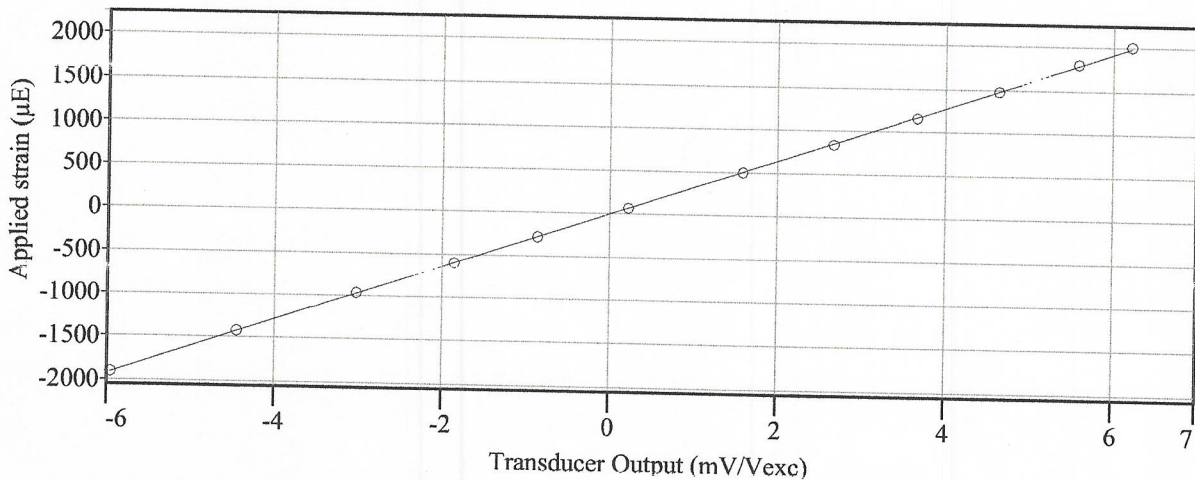

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: X779

Calibration Date: _____

FEB 02 2023

