




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 254C
 PDI Gage Factor: 110.0
 Mean Linear Correlation Coefficient: 0.999984

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2263.8	-5.888	774.3	2.070
-1758.5	-4.577	1255.5	3.345
-1286.1	-3.336	1719.2	4.576
-794.0	-2.047	2171.9	5.773
-269.0	-0.678	2644.4	6.962
269.0	0.721		

Calibration Curve

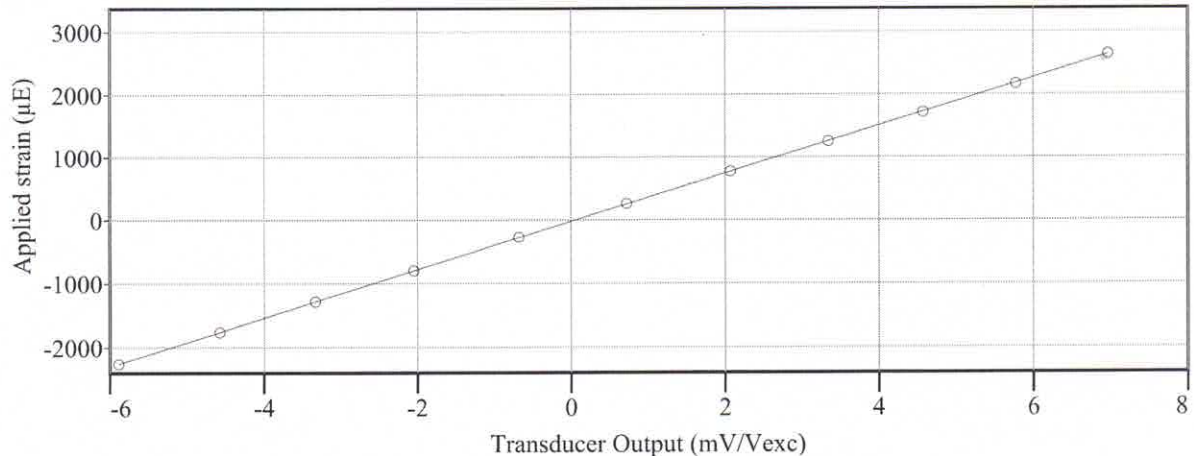

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: 254C

Calibration Date: 9/7/2023 8:04:42 AM

