




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: 262C  
 PDI Gage Factor: 110.0  
 Mean Linear Correlation Coefficient: 0.999915

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-2296.6	-5.915	794.0	2.300
-1804.5	-4.543	1305.8	3.632
-1325.5	-3.244	1771.7	4.883
-820.2	-1.907	2237.5	6.070
-288.7	-0.516	2683.7	7.199
255.9	0.900		

Calibration Curve

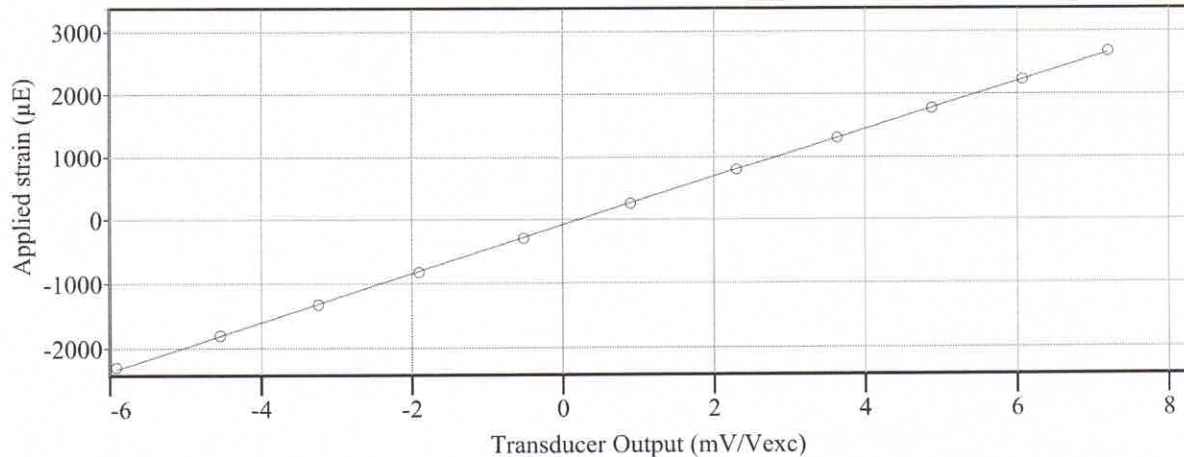

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: 262C

Calibration Date: 9/7/2023 8:00:58 AM

