




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 3995
 PDI Gage Factor: 86.9
 Mean Linear Correlation Coefficient: 0.999922

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2027.6	-6.652	564.3	1.935
-1496.1	-4.963	925.2	3.168
-1049.9	-3.477	1305.8	4.426
-636.5	-2.067	1666.7	5.606
-203.4	-0.645	2021.0	6.692
210.0	0.708		

Calibration Curve

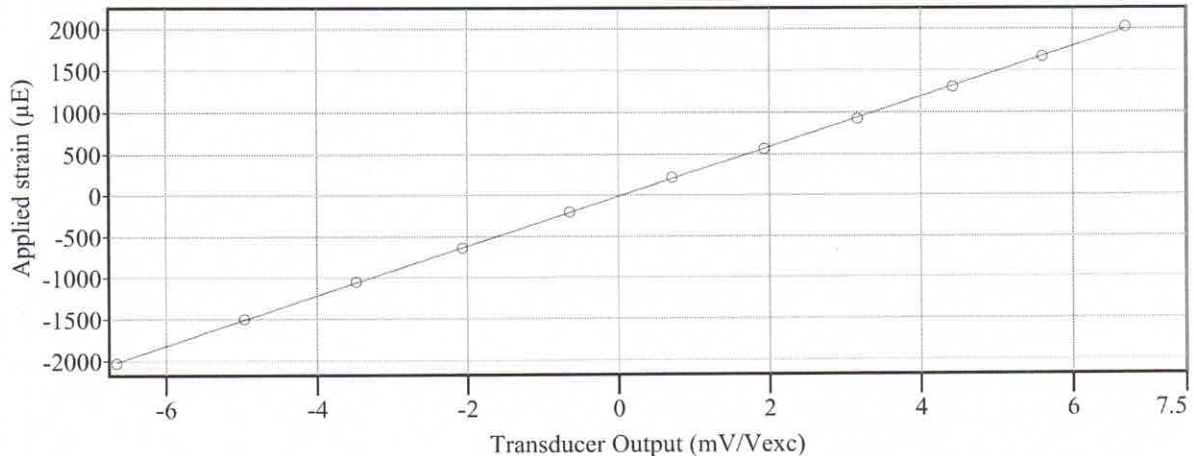

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: 3995

Calibration Date: 9/7/2023 7:43:36 AM

