




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: C149  
 PDI Gage Factor: 88.1  
 Mean Linear Correlation Coefficient: 0.999900

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-1929.1	-6.175	623.4	2.130
-1408.6	-4.550	951.4	3.248
-951.4	-3.076	1279.5	4.355
-562.1	-1.768	1633.9	5.455
-164.0	-0.453	1981.6	6.527
251.5	0.889		

Calibration Curve

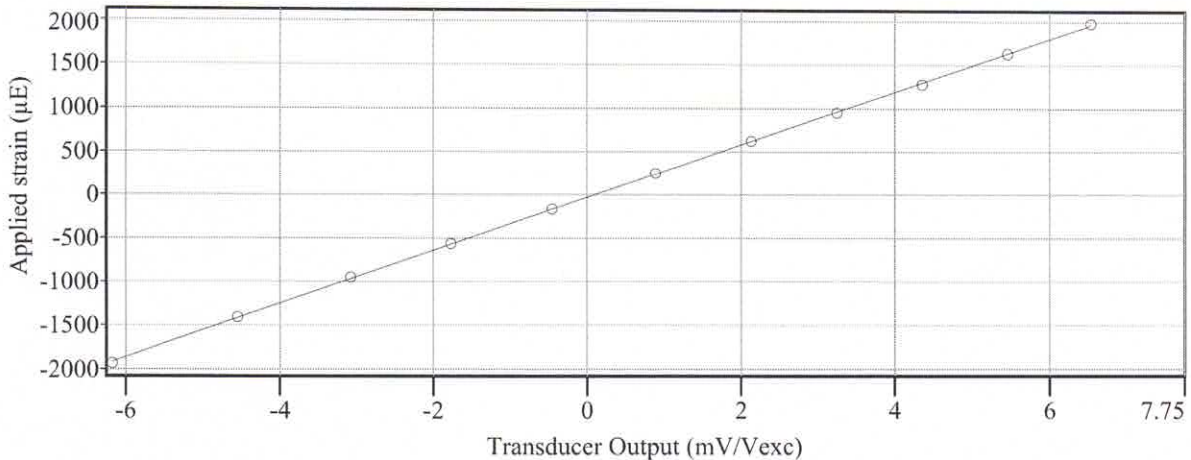

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: \_\_\_\_\_

*Paul Hartman*

PDI Gage: C149

Calibration Date: 6/6/2023 7:37:41 AM

