




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: C850  
 PDI Gage Factor: 90.0  
 Mean Linear Correlation Coefficient: 0.999956

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-2080.1	-6.540	708.7	2.323
-1555.1	-4.914	1122.0	3.684
-1115.5	-3.485	1496.1	4.922
-682.4	-2.100	1876.6	6.160
-229.7	-0.651	2290.0	7.443
249.3	0.843		

Calibration Curve

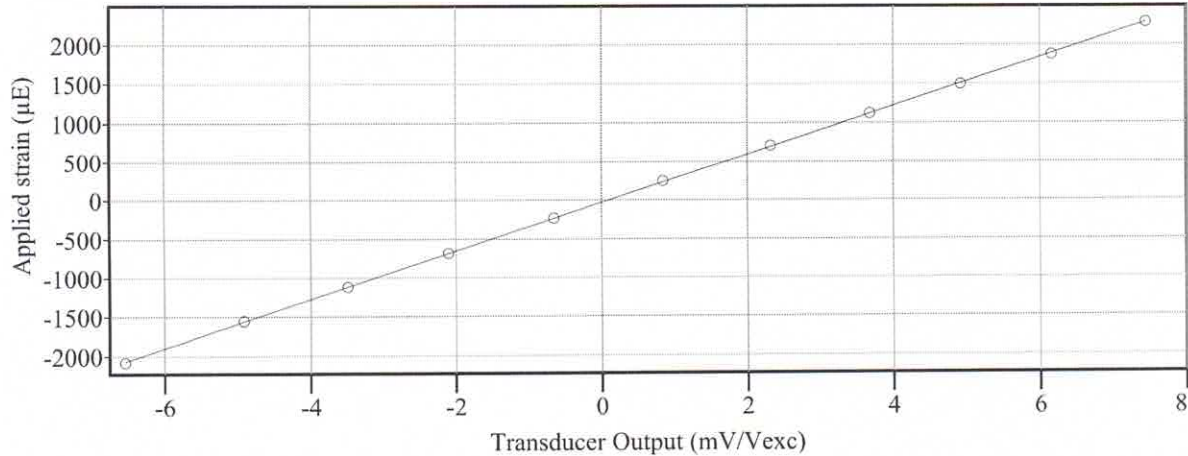

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: C850

Calibration Date: 9/7/2023 7:13:18 AM

