




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: G579
 PDI Gage Factor: 89.7
 Mean Linear Correlation Coefficient: 0.999832

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1876.6	-5.989	505.2	1.723
-1371.4	-4.423	859.6	2.869
-931.8	-3.029	1213.9	3.995
-551.2	-1.771	1542.0	5.021
-164.0	-0.484	1889.8	6.063
183.7	0.661	2021.0	6.448

Calibration Curve

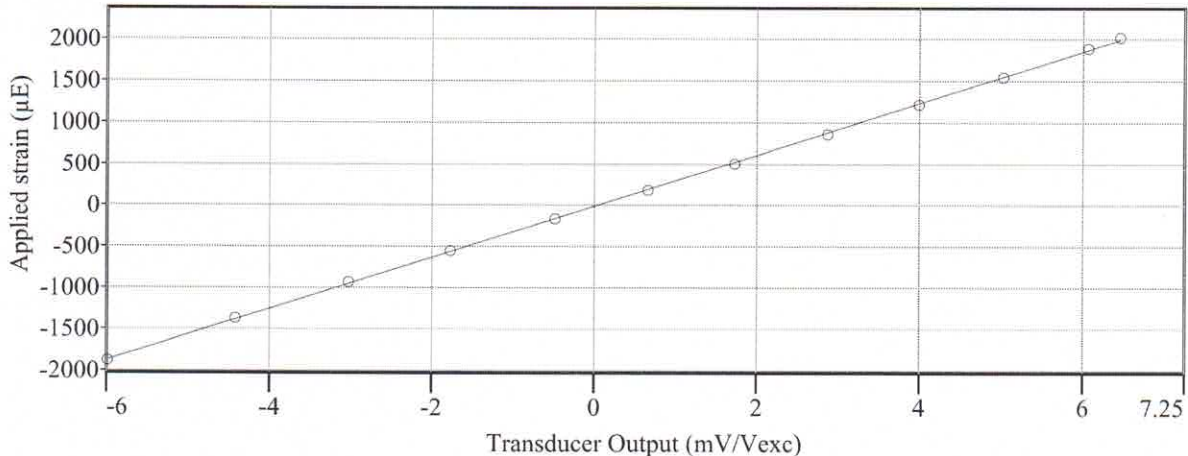

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: G579

Calibration Date: 6/6/2023 12:22:03 PM

