




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: J454  
 PDI Gage Factor: 91.5  
 Mean Linear Correlation Coefficient: 0.999875

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-1922.6	-6.045	301.8	1.101
-1522.3	-4.712	794.0	2.623
-1108.9	-3.358	1213.9	3.958
-675.9	-1.977	1627.3	5.240
-196.9	-0.466	2053.8	6.515

Calibration Curve

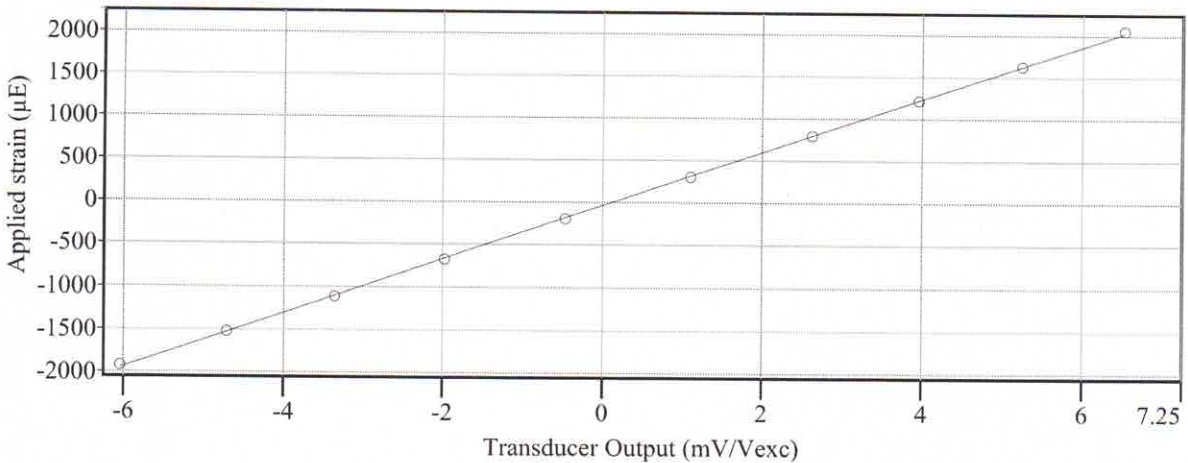

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: \_\_\_\_\_

PDI Gage: J454

Calibration Date: 6/8/2023 10:21:35 AM

