




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: J604
 PDI Gage Factor: 90.0
 Mean Linear Correlation Coefficient: 0.999936

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1994.8	-6.317	485.6	1.644
-1476.4	-4.695	826.8	2.757
-990.8	-3.168	1161.4	3.823
-577.4	-1.822	1478.6	4.815
-177.2	-0.549	1791.3	5.780
150.9	0.553	2001.3	6.439

Calibration Curve

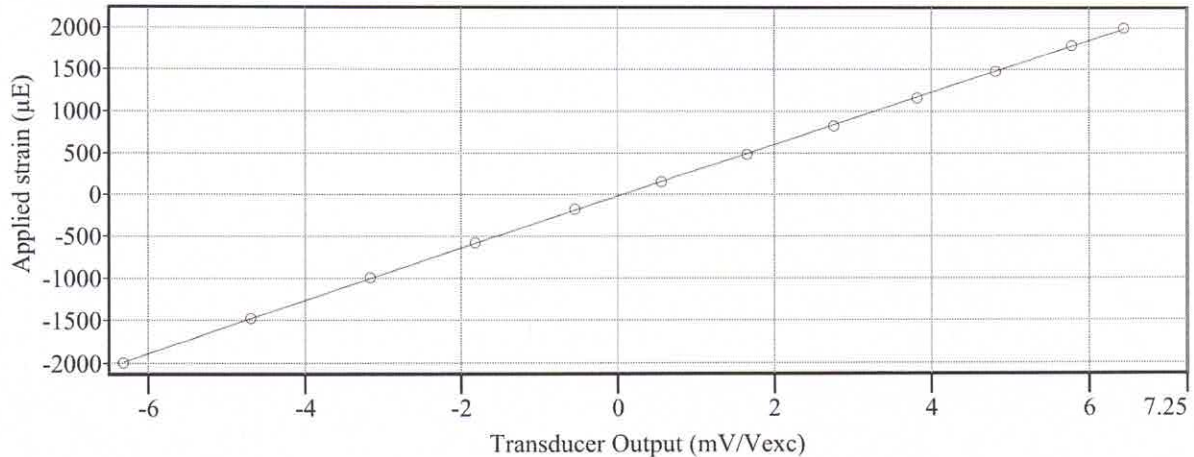

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: J604

Calibration Date: 9/12/2023 1:42:49 PM

