




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: P118
 PDI Gage Factor: 96.4
 Mean Linear Correlation Coefficient: 0.999768

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2290.0	-6.861	288.7	1.060
-1758.5	-5.194	813.6	2.580
-1240.2	-3.589	1308.0	4.024
-734.9	-2.038	1732.3	5.233
-229.7	-0.487	2040.7	6.159

Calibration Curve

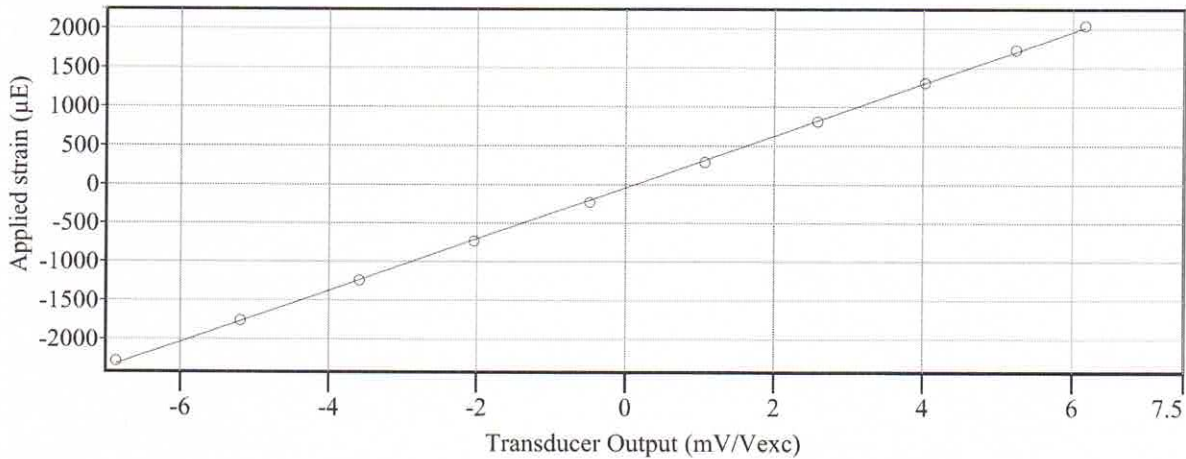

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: P118

Calibration Date: 6/8/2023 10:06:18 AM

