




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: T607  
 PDI Gage Factor: 140.5  
 Mean Linear Correlation Coefficient: 0.999968

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-2021.0	-4.142	597.1	1.242
-1502.6	-3.126	977.7	2.018
-1082.7	-2.233	1371.4	2.822
-662.7	-1.361	1765.1	3.631
-223.1	-0.452	2152.2	4.400
223.1	0.446		

Calibration Curve

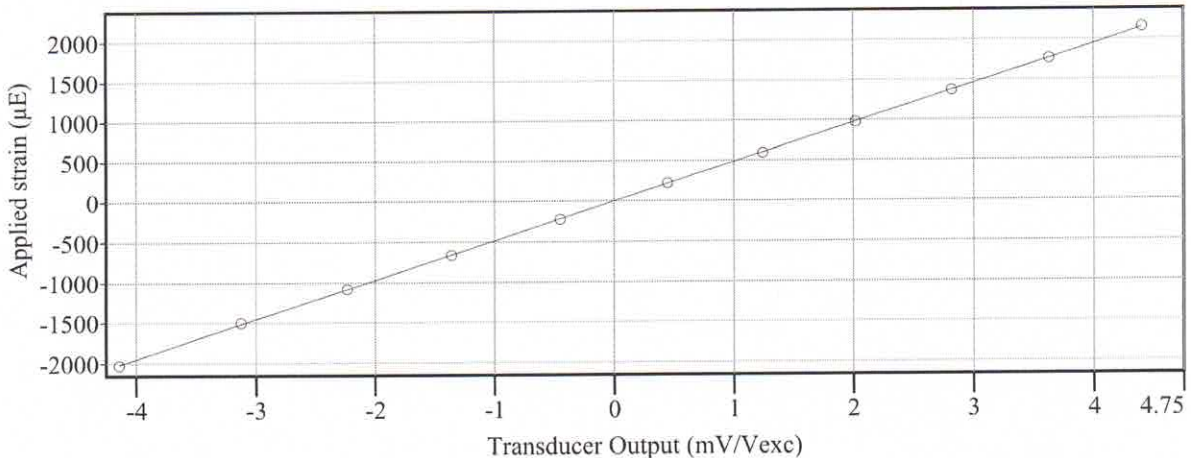

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: T607

Calibration Date: 9/7/2023 7:24:54 AM

