




# Certificate of Calibration

TechSense  
 Transducer Model: PDI Strain Transducer  
 Serial Number: V415  
 PDI Gage Factor: 138.2  
 Mean Linear Correlation Coefficient: 0.999796

Table 1: Representative Calibration Data

Applied strain ( $\mu E$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu E$ )	Gage Output (mV/Vexc)
-1987.6	-4.460	436.3	0.812
-1430.4	-3.308	927.6	1.906
-940.7	-2.267	1328.5	2.781
-657.1	-1.645	1716.5	3.589
-141.1	-0.495	2105.0	4.362
203.2	0.285		

Calibration Curve

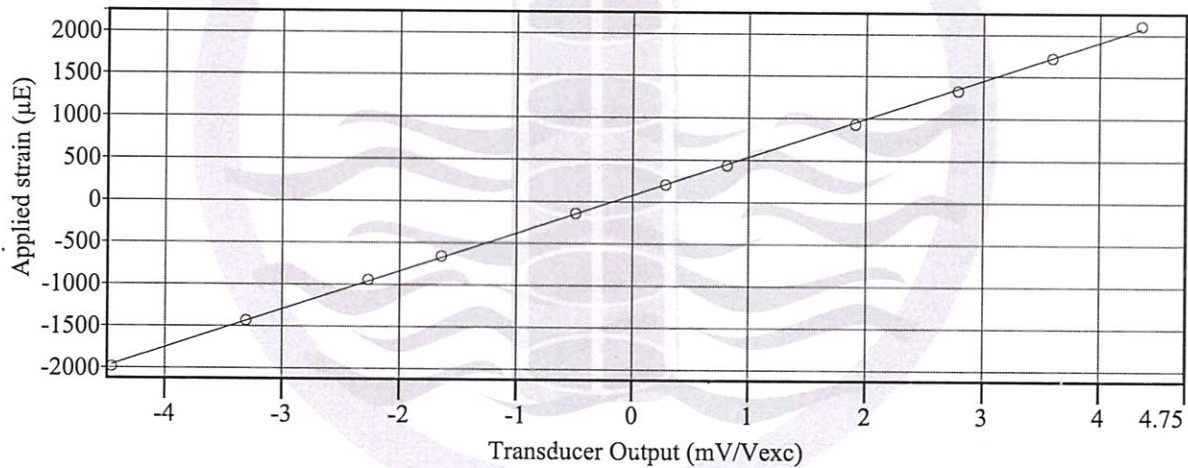

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1003HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: RASENDU PATEL

Signature: \_\_\_\_\_

PDI Gage: V415

Calibration Date: 13-02-2023 17:42:47



## TechSense

49, Atmajyoti Nagar Society, Near Atmajyoti Ashram, Ellora Park, Vadodara - 390023  
 Website : [www.techsenseindia.com](http://www.techsenseindia.com) E-mail : [info@techsenseindia.com](mailto:info@techsenseindia.com)  
 Mobile.: +91- 8905510013 / +91 9327226069