



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: L331


PDI Gage Factor: 89.9

Mean Linear Correlation Coefficient: 0.999747

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2316.3	-7.099	387.1	1.590
-1784.8	-5.419	702.1	2.632
-1246.7	-3.741	1030.2	3.686
-721.8	-2.102	1345.1	4.662
-216.5	-0.516	1653.5	5.602
131.2	0.666	2034.1	6.722

Calibration Curve

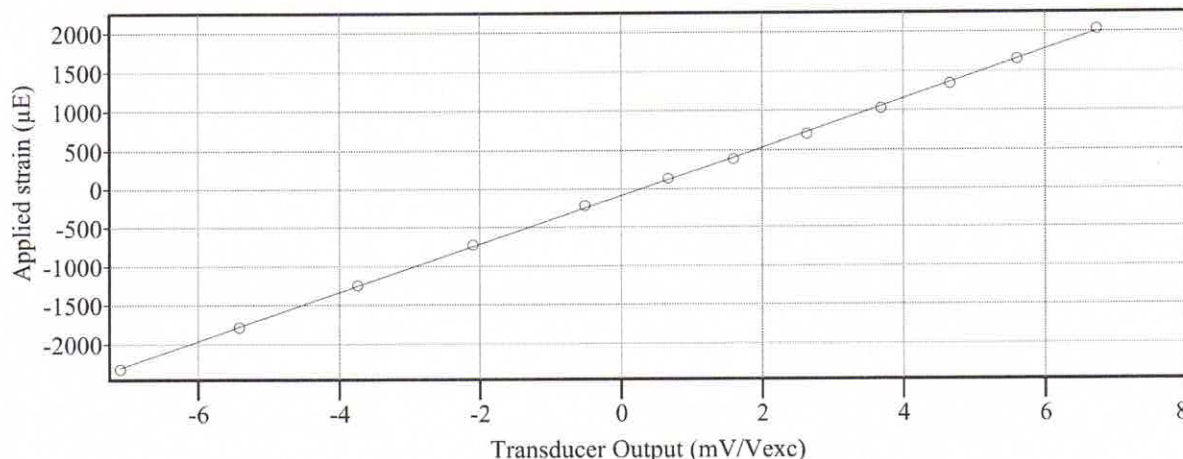

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: L331

Calibration Date: 1/16/2024 10:48:26 AM

