




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 6583
PDI Gage Factor: 94.5
Mean Linear Correlation Coefficient: 0.999875

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1875.0	-5.711	475.0	1.555
-1341.7	-4.067	808.3	2.593
-833.3	-2.491	1175.0	3.669
-341.7	-0.988	1533.3	4.711
125.0	0.422	1925.0	5.858

Calibration Curve

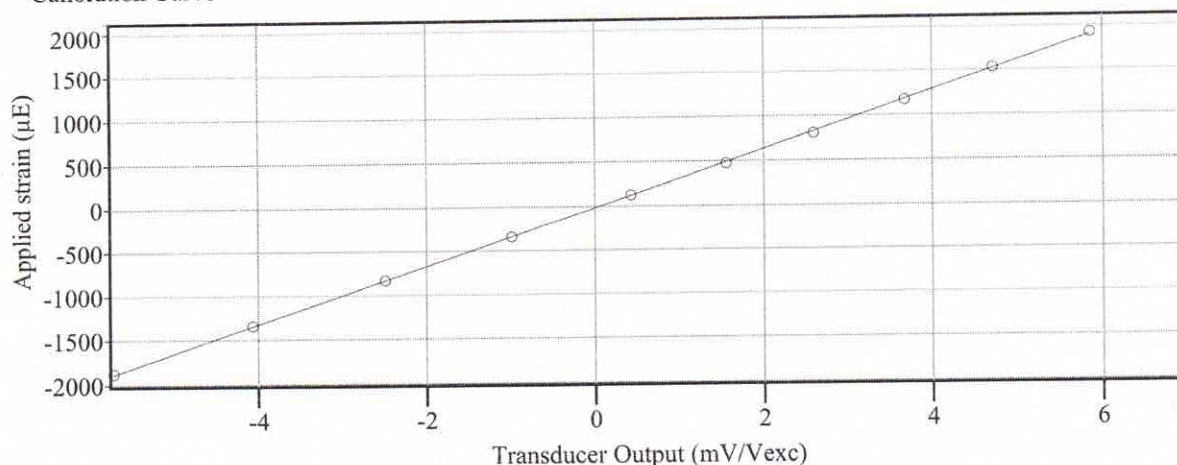

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: 6583

Calibration Date: 4/10/2024 9:18:44 AM

