



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: C437


PDI Gage Factor: 94.5

Mean Linear Correlation Coefficient: 0.999512

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1833.3	-5.570	288.9	1.013
-1283.3	-3.919	558.3	1.831
-766.7	-2.311	813.9	2.595
-275.0	-0.842	1050.0	3.273
41.7	0.205	1625.0	4.858

Calibration Curve

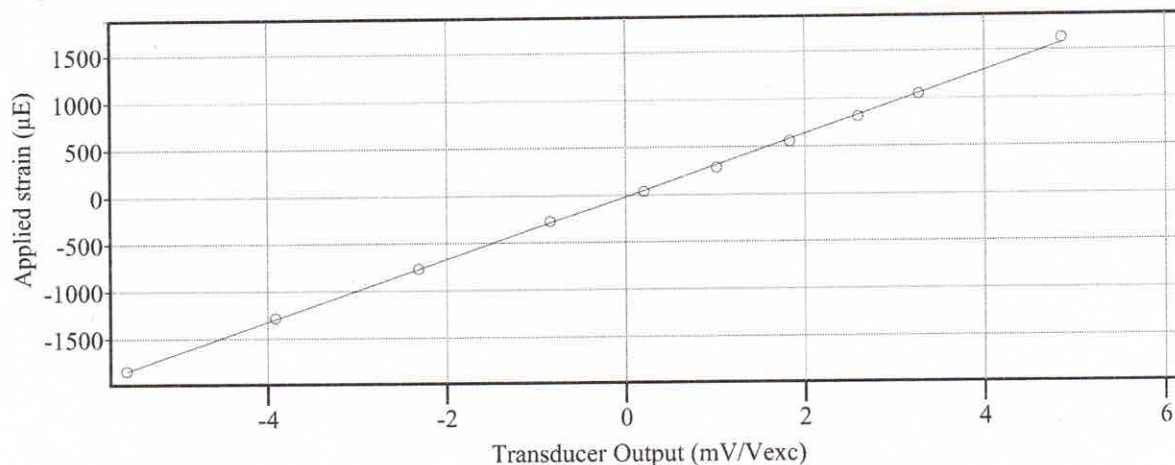

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: C437

Calibration Date: 4/10/2024 9:29:44 AM

