



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: Z777


PDI Gage Factor: 95.1

Mean Linear Correlation Coefficient: 0.999862

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1141.7	-3.471	643.0	2.023
-734.9	-2.197	964.6	2.987
-374.0	-1.124	1259.8	3.885
-85.3	-0.222	1935.7	5.844
242.8	0.803		

Calibration Curve

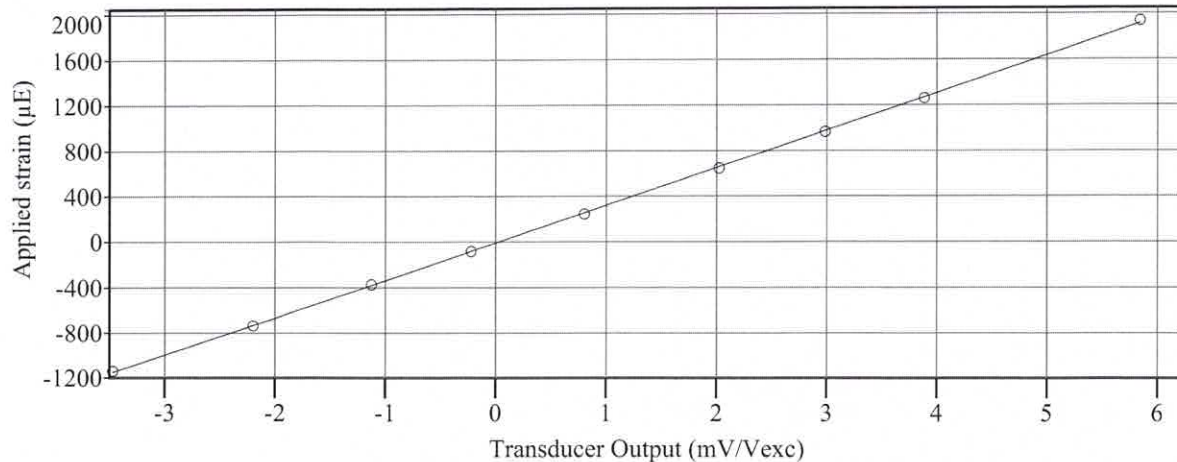

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: Z777

Calibration Date: APR 05 2024

