



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: X386


PDI Gage Factor: 91.7

Mean Linear Correlation Coefficient: 0.999981

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2257.2	-6.832	485.6	1.779
-1745.4	-5.223	787.4	2.774
-1227.0	-3.596	1082.7	3.709
-721.8	-2.024	1378.0	4.616
-295.3	-0.669	1660.1	5.510
105.0	0.591	1988.2	6.496

Calibration Curve

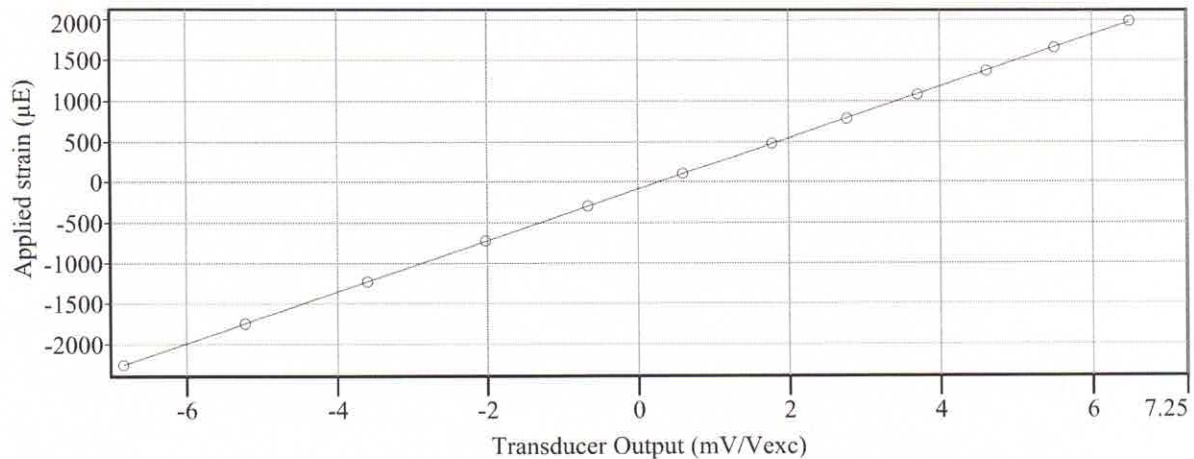

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: X386

Calibration Date: 6/5/2024 7:06:50 AM

