



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: X389


PDI Gage Factor: 90.0

Mean Linear Correlation Coefficient: 0.999765

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2276.9	-7.182	393.7	1.425
-1745.4	-5.534	721.8	2.491
-1220.5	-3.882	1036.7	3.466
-702.1	-2.240	1351.7	4.427
-210.0	-0.705	1686.4	5.468
91.9	0.379	2027.6	6.489

Calibration Curve

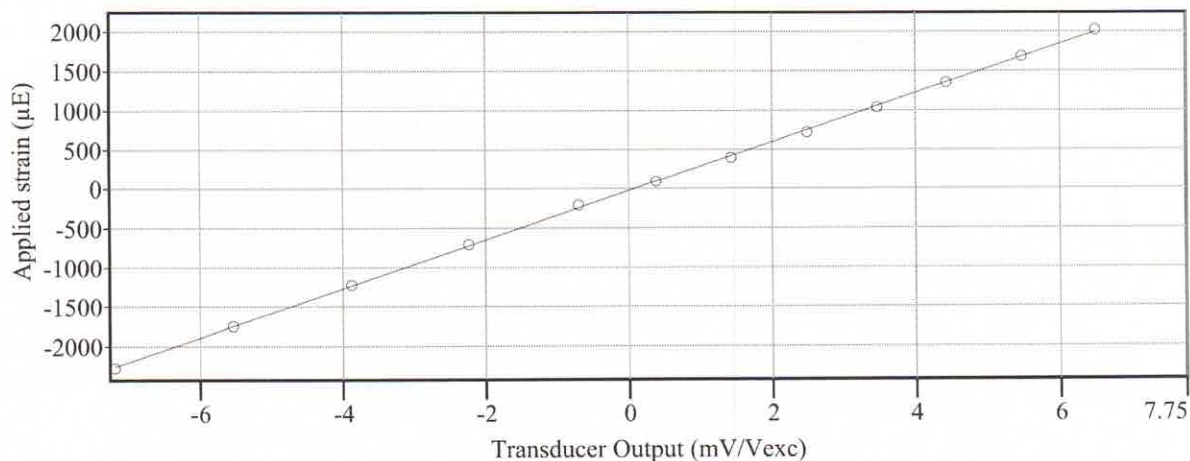

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: X389

Calibration Date: 6/5/2024 7:56:37 AM

