



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: Z896


PDI Gage Factor: 95.9

Mean Linear Correlation Coefficient: 0.999985

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2972.4	-8.732	492.1	1.695
-2270.3	-6.616	990.8	3.230
-1587.9	-4.564	1417.3	4.525
-958.0	-2.676	1850.4	5.778
-393.7	-0.988	2001.3	6.223
19.7	0.259		

Calibration Curve

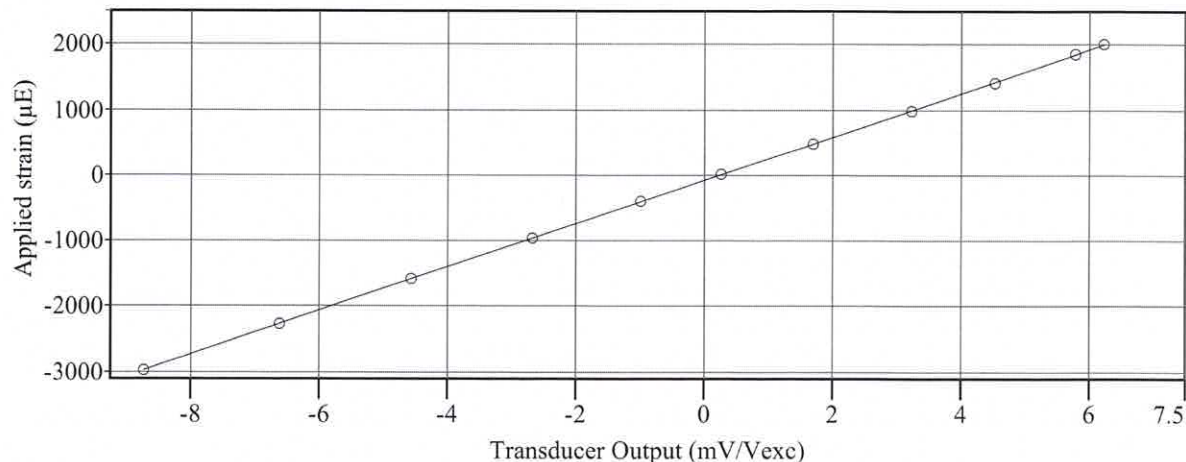

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

PDI Gage: Z896

Calibration Date: _____

Signature: _____

Paul Hartman

MAY 24 2024

