



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: Z913


PDI Gage Factor: 98.8

Mean Linear Correlation Coefficient: 0.999974

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2952.8	-8.319	472.4	1.724
-2263.8	-6.286	964.6	3.173
-1587.9	-4.324	1391.1	4.412
-958.0	-2.502	1811.0	5.598
-406.8	-0.913	1994.8	6.120
-6.6	0.305		

Calibration Curve

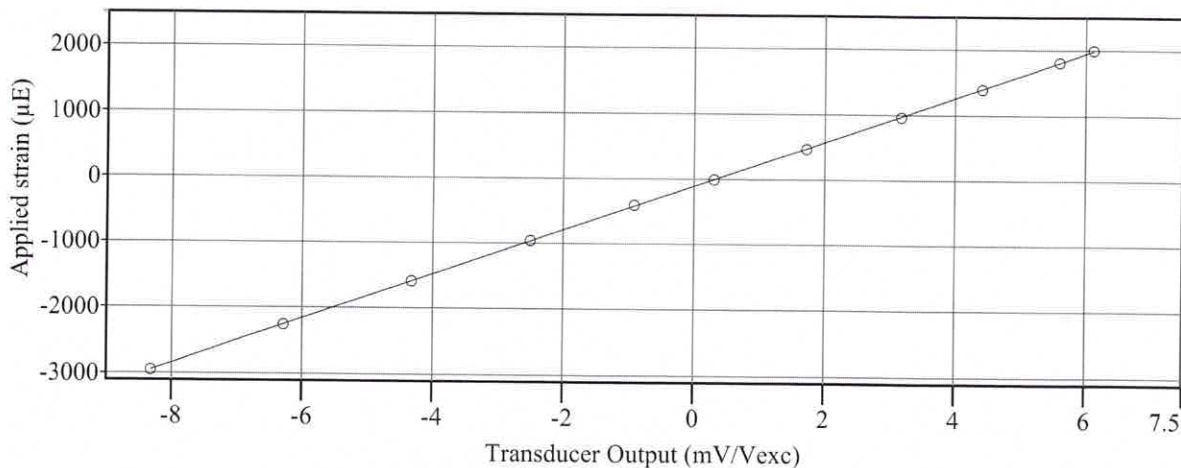

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: VANNA OUK

Signature: _____

PDI Gage: Z913

Calibration Date: MAY 14 2024

