



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: G042


PDI Gage Factor: 98.1

Mean Linear Correlation Coefficient: 0.999706

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1961.9	-5.715	500.9	1.683
-1456.7	-4.224	853.0	2.684
-984.3	-2.820	1185.5	3.644
-544.6	-1.507	1528.9	4.607
-155.3	-0.322	1870.1	5.563
164.0	0.688	2021.0	5.942

Calibration Curve

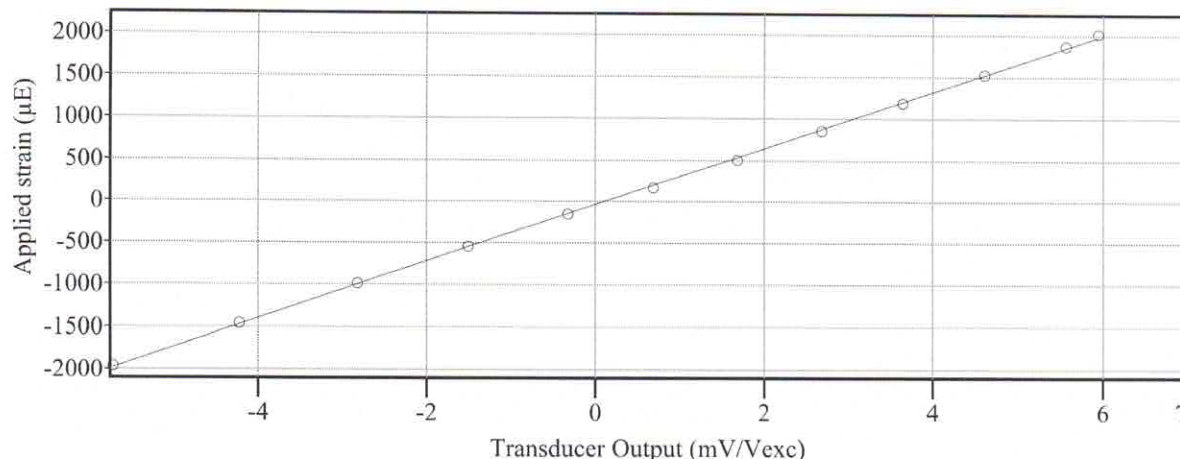

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: G042

Calibration Date: 6/28/2024 8:20:35 AM

