




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: J187
 PDI Gage Factor: 94.5
 Mean Linear Correlation Coefficient: 0.999965

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2388.5	-7.034	551.2	1.997
-1857.0	-5.413	958.0	3.221
-1332.0	-3.810	1292.7	4.244
-820.2	-2.220	1614.2	5.205
-334.6	-0.725	2093.2	6.614
118.1	0.664		

Calibration Curve

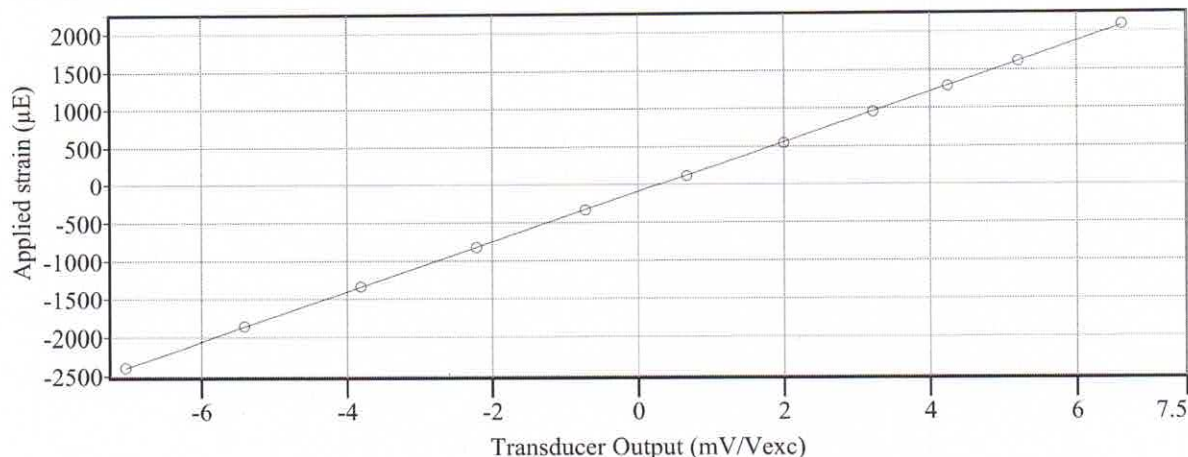

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: J187

Calibration Date: _____

