



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: W541


PDI Gage Factor: 91.2

Mean Linear Correlation Coefficient: 0.999773

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1824.1	-5.479	577.4	2.246
-1338.6	-3.939	918.6	3.308
-879.3	-2.458	1240.2	4.299
-465.9	-1.127	1607.6	5.393
-118.1	0.012	1975.1	6.487
223.1	1.119		

Calibration Curve

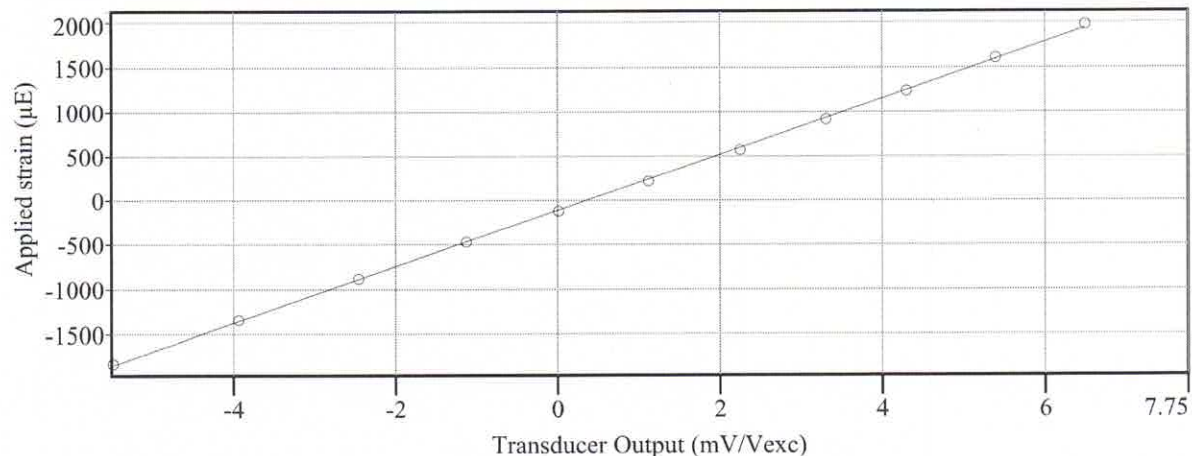

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: W541

Calibration Date: 7/1/2024 8:25:31 AM

