




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: E583
 PDI Gage Factor: 90.9
 Mean Linear Correlation Coefficient: 0.999798

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2126.0	-6.482	446.2	1.757
-1614.2	-4.862	754.6	2.735
-1089.2	-3.227	1034.6	3.629
-577.4	-1.615	1312.3	4.479
-137.8	-0.220	1603.2	5.348
150.9	0.792	2066.9	6.722

Calibration Curve

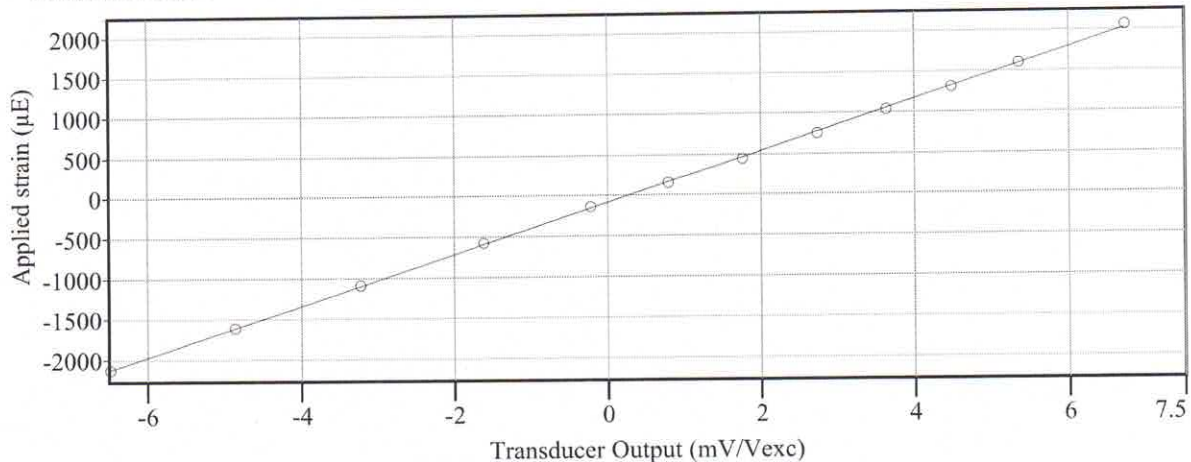

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: E583

Calibration Date: 7/1/2024 9:50:29 AM

