

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K4021 Temperature: 25.5 °C
Model: KICHER PR Humidity: 60%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

407.9 mv/5000g
(81.6 $\mu\text{v/g}$)
R²: 0.999907 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 01Aug2024

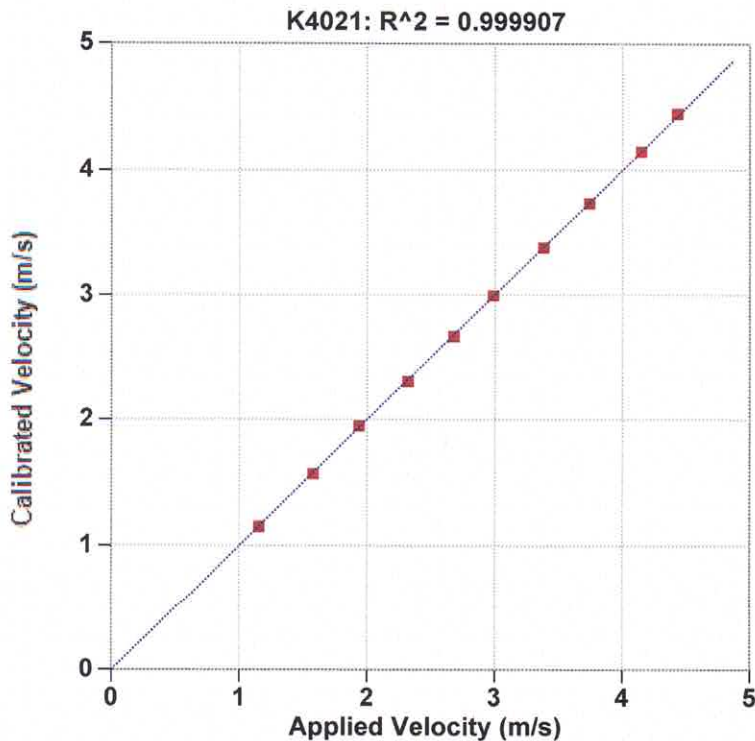

Reference Velocity	S/N K4021 Velocity
m/s	m/s
1.159	1.156
1.581	1.572
1.941	1.951
2.323	2.307
2.683	2.670
2.991	2.997
3.387	3.382
3.746	3.740
4.150	4.152
4.434	4.452
Maximum Acceleration: 954 g's	