

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 22538 Temperature: 24.3 °C
Model: PE Humidity: 44%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1061.9 g's/volt

R^2: 0.999971 [No chip]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 19Aug2024

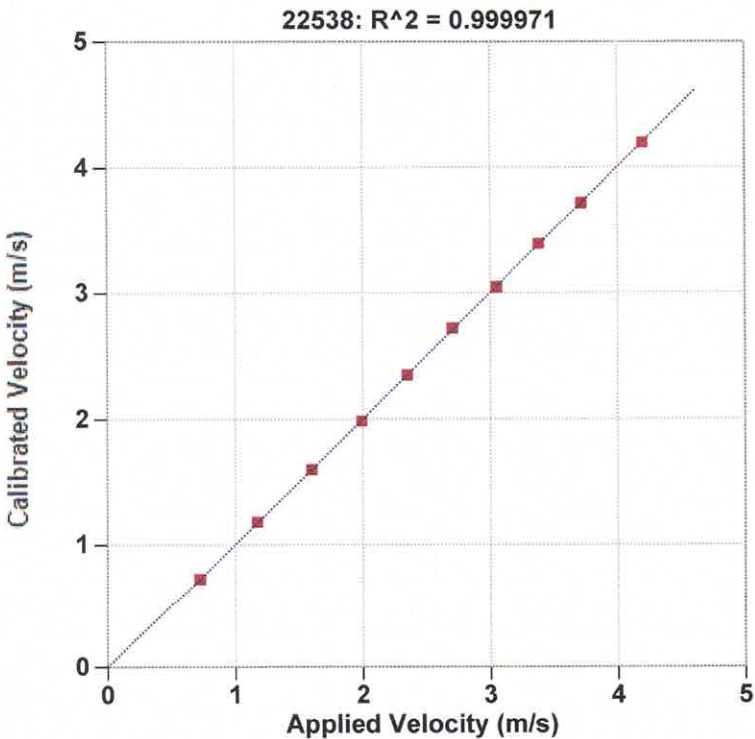

Reference Velocity	S/N 22538 Velocity
m/s	m/s
0.726	0.726
1.179	1.184
1.605	1.604
1.996	1.988
2.355	2.353
2.710	2.722
3.056	3.049
3.386	3.391
3.723	3.723
4.203	4.199
Maximum Acceleration: 904 g's	