


Serial Number 30388
Force Calibration (kips/mV/V) -17.6251251
Offset 0.0043723
Correlation -0.99999597

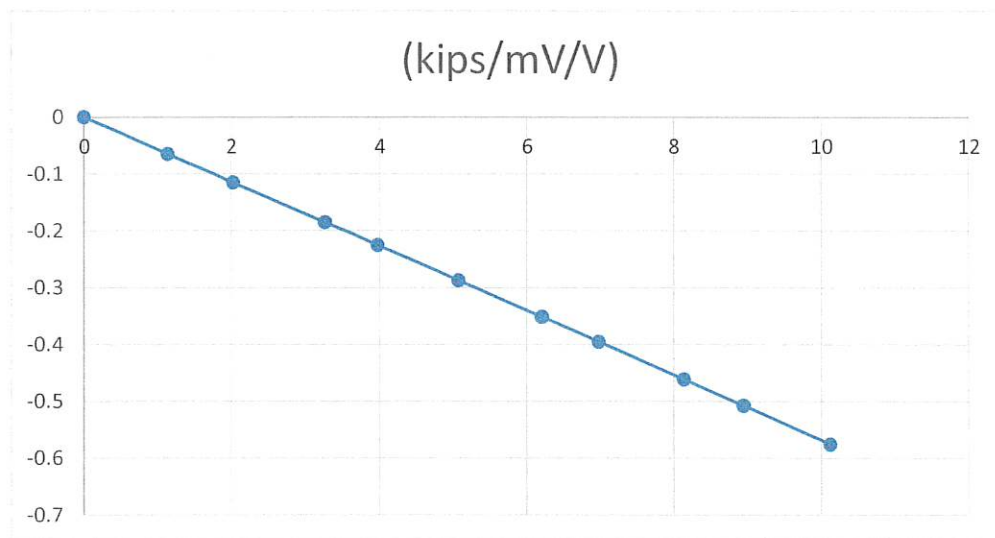

Serial Number 30388
Force Calibration (kips/mV/V) -17.6166212
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3523.32423

Calibrated by: Sam Boney
Calibrated Date: 9/3/2024


Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.10021929	-0.062828302
3 1.97711925	-0.11177641
4 2.9220577	-0.165762009
5 3.95394508	-0.223543518
6 5.05884222	-0.286116123
7 6.18957048	-0.349456499
8 6.94988768	-0.393718034
9 8.12087357	-0.459518037
10 8.91628225	-0.503590106
11 9.92038823	-0.568352424

Serial Number 30388
Force Calibration (lb/V) -17.5750246
Offset 0.01931836
Correlation -0.99992476

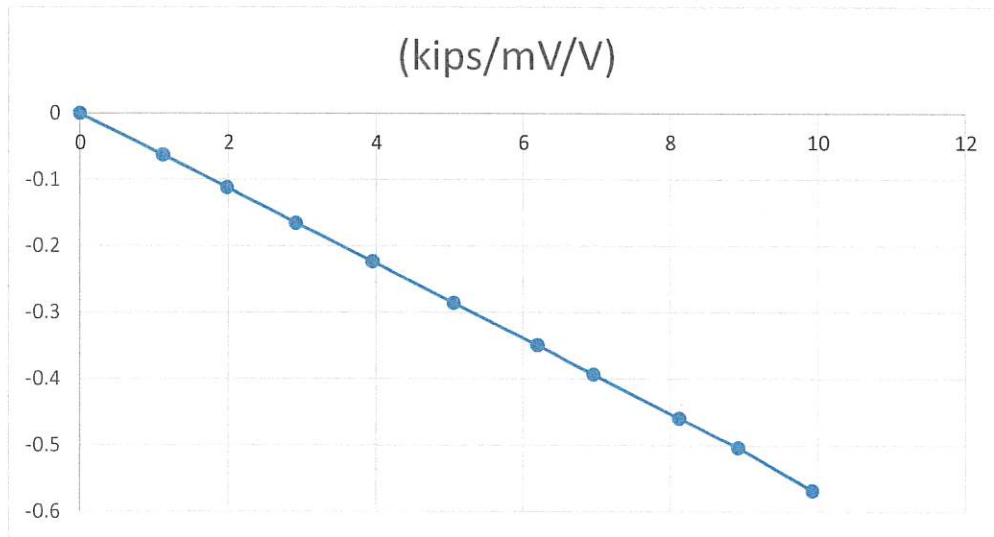


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.86851723	-0.049635216
3 2.00577735	-0.113833114
4 3.00832445	-0.170282958
5 4.05015442	-0.229187605

6	5.14715593	-0.291684408
7	5.90942274	-0.335073946
8	7.06500741	-0.399897676
9	7.840141	-0.444737413
10	8.97301351	-0.512992267
11	9.92808879	-0.559007362

Serial Number 30388
 Force Calibration (kips/mV/V) -17.6497138
 Offset -0.00302673
 Correlation -0.99993544

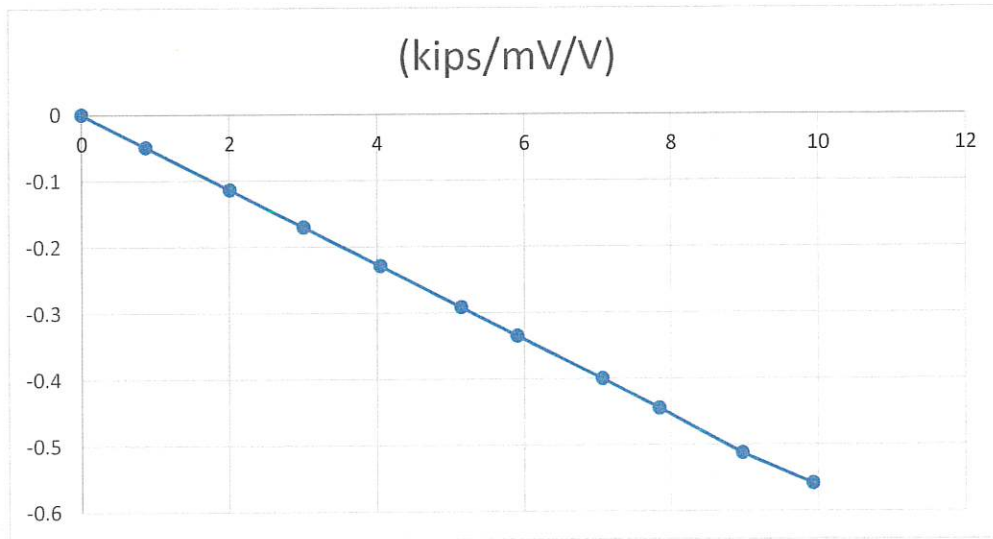

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.13755288	-0.064572344
3	2.02205603	-0.114861668
4	3.26663761	-0.185092399
5	3.9687616	-0.224946718
6	5.07200166	-0.287097713
7	6.19707629	-0.351092226
8	6.97669385	-0.395126413
9	8.13695732	-0.46103086
10	8.94727992	-0.507155024
11	10.1202153	-0.575045256