


Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.85214114	-0.048057126
3 1.99057097	-0.113709813
4 2.90041781	-0.164733563
5 4.0833939	-0.232281919
6 4.7808389	-0.27233044
7 5.99890619	-0.34166548
8 6.76146536	-0.385590508
9 8.12798922	-0.461342189
10 8.85019301	-0.508091715
11 9.89007289	-0.571195349

Serial Number 30391
Force Calibration (lb/V) -17.377024
Offset 0.0384625
Correlation -0.99991904

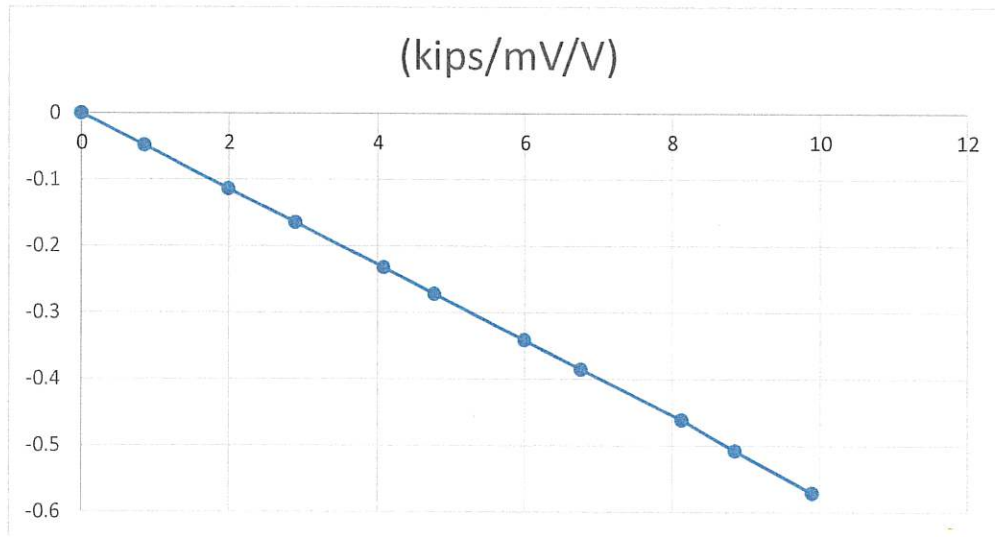


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.82523758	-0.047479233
3 1.92604143	-0.109601788
4 2.82233903	-0.161161337
5 3.84262669	-0.218682519


6	4.93748375	-0.280094441
7	6.08497798	-0.346382824
8	6.85933181	-0.390023834
9	8.05936571	-0.458549172
10	8.85038794	-0.504602432
11	9.91142023	-0.566081106

Serial Number 30391
 Force Calibration (kips/mV/V) -17.5410705
 Offset 0.00460789
 Correlation -0.99999106

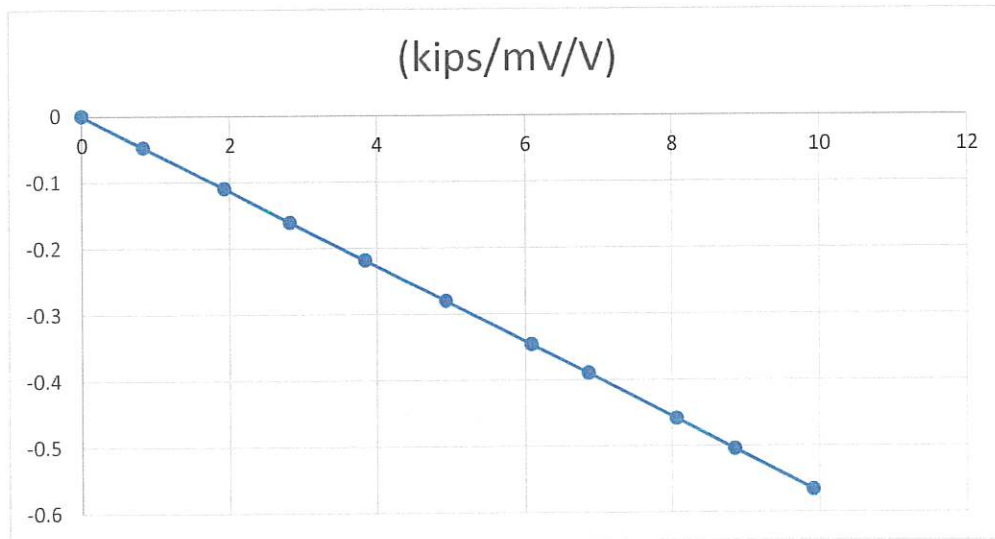

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.1499324	-0.065871345
3	2.03930936	-0.116317487
4	3.1468388	-0.178904906
5	4.24832443	-0.241700933
6	4.88582132	-0.277304822
7	6.03302315	-0.342517885
8	7.21063753	-0.410005775
9	8.00458408	-0.455059379
10	9.21914195	-0.524158743
11	10.1475086	-0.577899103

Serial Number 30391
Force Calibration (kips/mV/V) -17.5856167
Offset -0.000843
Correlation -0.99999685

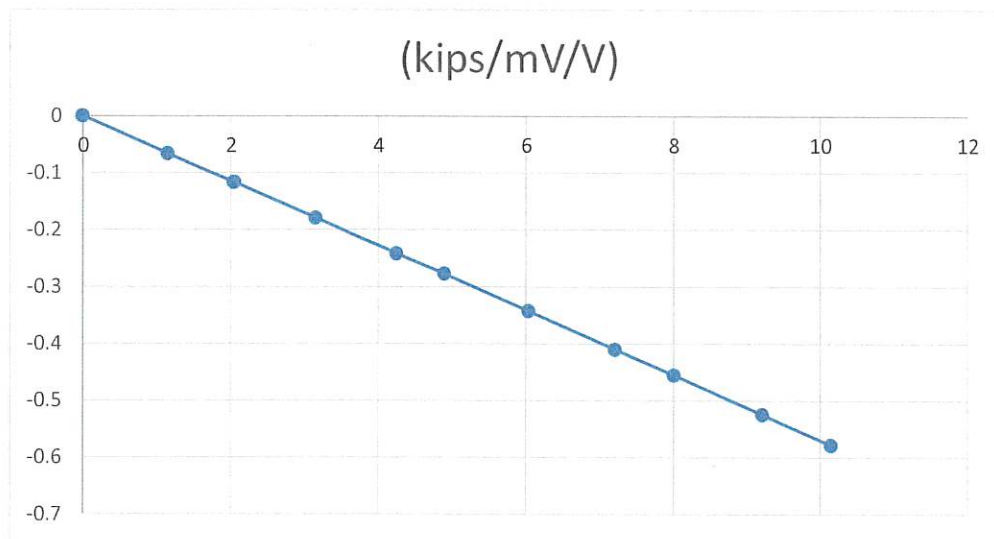

Serial Number 30391
Force Calibration (kips/mV/V) -17.501237

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3500.24741

Calibrated by: Jean Bonner
Calibrated Date: 9/4/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

