


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.86286357	-0.048806036
3	2.06923461	-0.115856939
4	3.08533094	-0.173136261
5	3.79895718	-0.214033174
6	4.87509874	-0.274753063
7	6.00738663	-0.338003616
8	6.75551927	-0.381033184
9	7.95867242	-0.44782861
10	8.7287372	-0.491791853
11	9.92263003	-0.560445118

Serial Number 30393
Force Calibration (lb/V) -17.7164017
Offset 0.0105801
Correlation -0.99999443

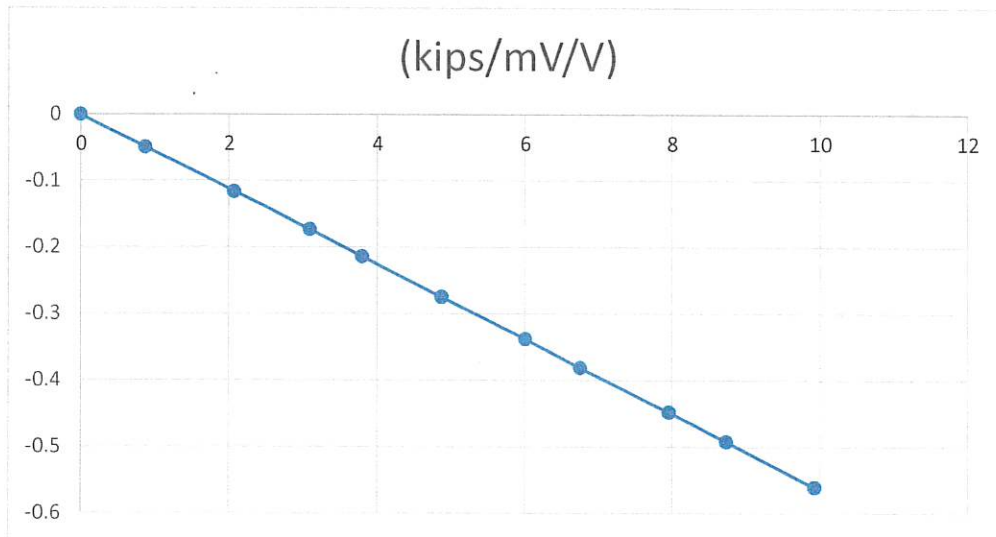


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.10723761	-0.062615328
3	1.99378776	-0.112302936
4	3.00159862	-0.169132157
5	4.0342658	-0.227634285


6	5.14267208	-0.290207233
7	5.8829092	-0.332028415
8	7.01529446	-0.395582467
9	8.20499584	-0.462975169
10	8.98919471	-0.506786881
11	10.21467	-0.575326596

Serial Number 30393
 Force Calibration (kips/mV/V) -17.7448307
 Offset -0.00361688
 Correlation -0.99999875

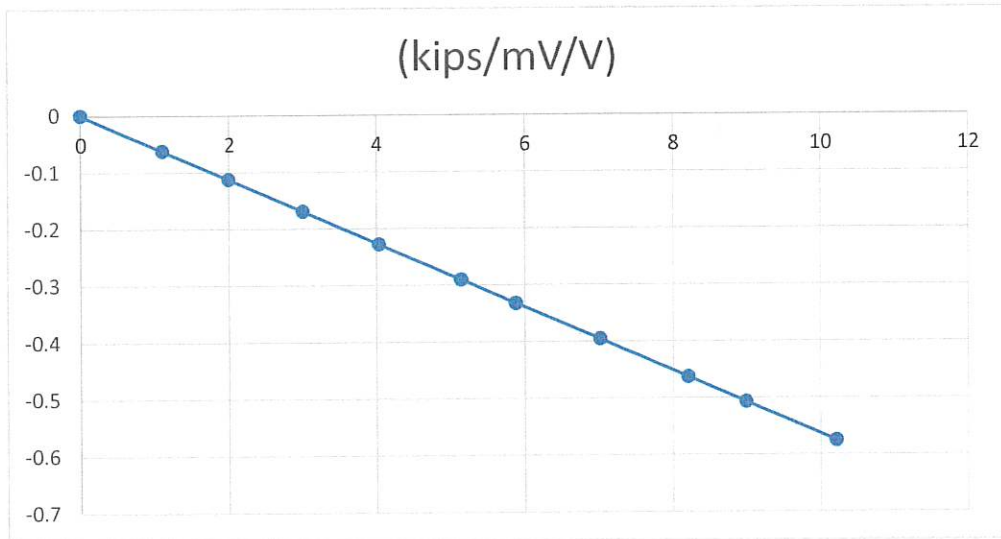

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	0.96141253	-0.054170569
3	2.1531621	-0.122003512
4	3.08201688	-0.174828344
5	4.13349703	-0.234164529
6	5.22367519	-0.295268411
7	5.96820127	-0.337094334
8	7.13743267	-0.403032084
9	7.90847225	-0.446208711
10	9.0956392	-0.513634663
11	10.0130885	-0.561171259

Serial Number 30393
Force Calibration (kips/mV/V) -17.7998357
Offset -0.02429464
Correlation -0.99997625

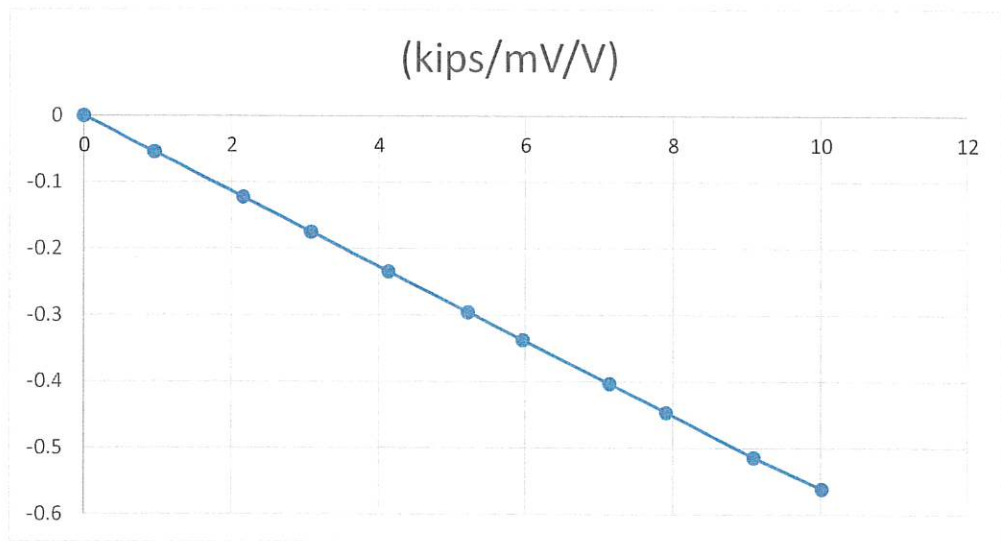

Serial Number 30393
Force Calibration (kips/mV/V) -17.7536894

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3550.73787

Calibrated by: Sean Benson
Calibrated Date: 7/30/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

