


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.86520303	-0.048649513
3	2.02478529	-0.114615003
4	2.92137531	-0.164875819
5	3.96759174	-0.224012651
6	5.07385354	-0.285438433
7	5.83329354	-0.327908602
8	7.00359718	-0.394334056
9	8.17994427	-0.459935018
10	8.85360474	-0.499334493
11	10.0082145	-0.571115167

Serial Number 30394
Force Calibration (lb/V) -17.6391053
Offset 0.02227693
Correlation -0.9999243

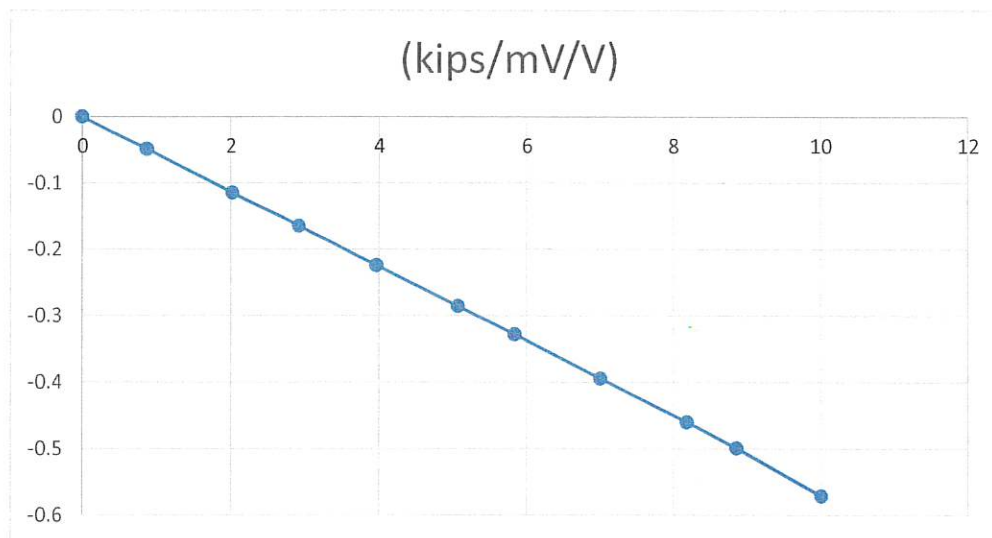


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.12371118	-0.063894544
3	1.98949881	-0.113259667
4	3.21799675	-0.182623007
5	4.25777969	-0.242219523


6	5.00600998	-0.284466928
7	6.13644583	-0.347655643
8	6.92932021	-0.392059334
9	8.08968115	-0.458636503
10	9.2294745	-0.526701784
11	10.1756794	-0.572754778

Serial Number 30394
 Force Calibration (kips/mV/V) -17.6819696
 Offset -0.01485982
 Correlation -0.99994488

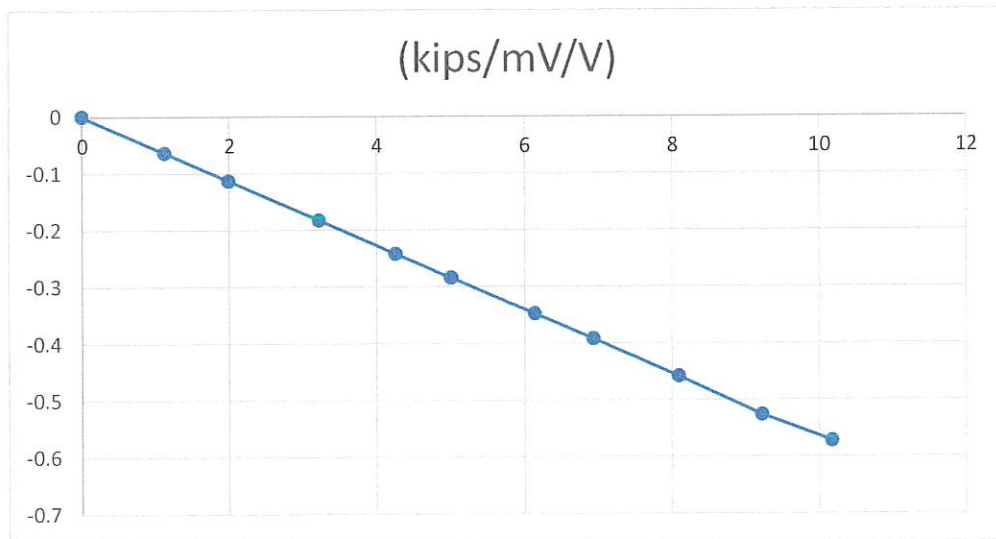

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	0.85155628	-0.048028721
3	2.02809948	-0.113799922
4	2.91084782	-0.164302426
5	3.96564218	-0.223074367
6	5.05864717	-0.285277336
7	5.81574773	-0.327652731
8	6.989658	-0.394106627
9	7.78535914	-0.437993822
10	8.99650533	-0.506703588
11	10.0723541	-0.57522389

Serial Number 30394
Force Calibration (kips/mV/V) -17.614803
Offset 0.02884044
Correlation -0.99992352

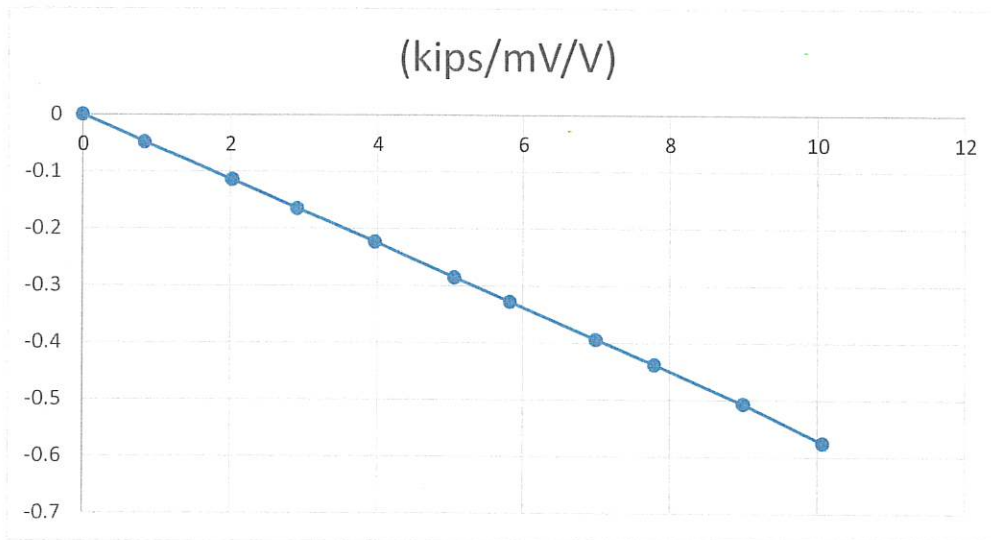

Serial Number 30394
Force Calibration (kips/mV/V) -17.6452926
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3529.05853

Calibrated by: *Sean Bonney*
Calibrated Date: 9/3/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

