




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 52A
PDI Gage Factor: 94.8
Mean Linear Correlation Coefficient: 0.999989

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2047.2	-6.058	393.7	1.417
-1542.0	-4.516	826.8	2.706
-1063.0	-3.045	1207.3	3.882
-662.7	-1.830	1548.6	4.916
-334.6	-0.840	1870.1	5.884
-6.6	0.169	1994.8	6.239

Calibration Curve

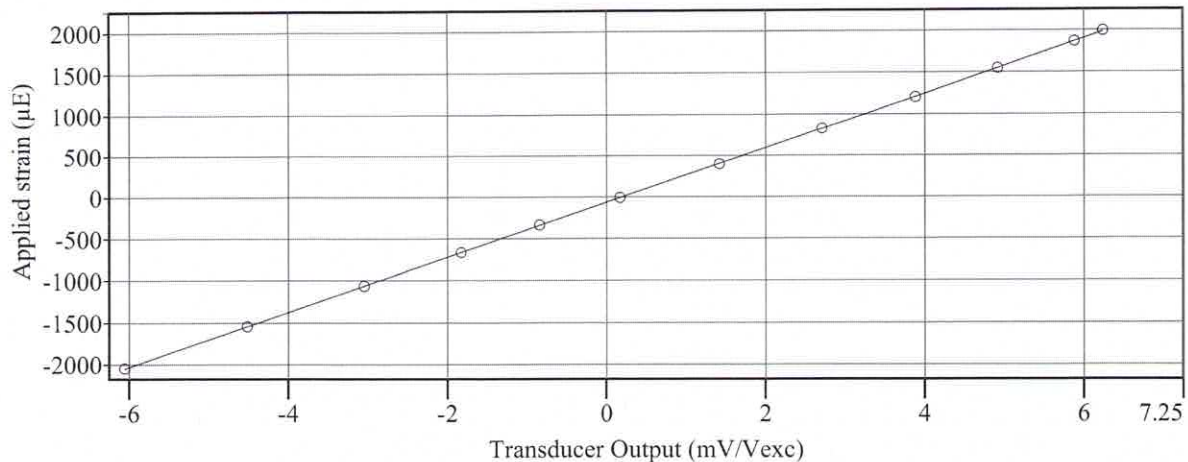

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: 52A

JUL 3 1 2024

Calibration Date: _____

