

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K973      Temperature: 23.6 °C  
Model: KICHER PR      Humidity: 40%  
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

319.8 mv/5000g  
(64.0 µv/g)  
R^2: 0.999983 [Chip programmed]

Ref Acc 1: 78270!      Cal on: 11Jan2024  
971 g's/volt  
Ref Acc 2: 78268!      Cal on: 11Jan2024  
986 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 20Aug2024

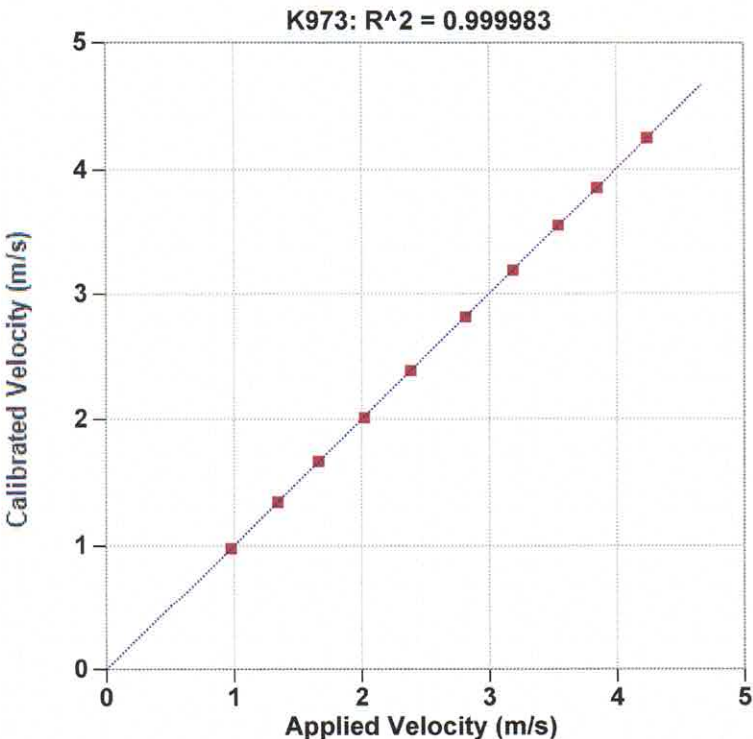

| Reference Velocity            | S/N K973 Velocity |
|-------------------------------|-------------------|
| m/s                           | m/s               |
| 0.980                         | 0.978             |
| 1.346                         | 1.344             |
| 1.665                         | 1.669             |
| 2.024                         | 2.012             |
| 2.389                         | 2.389             |
| 2.817                         | 2.815             |
| 3.192                         | 3.190             |
| 3.548                         | 3.548             |
| 3.852                         | 3.856             |
| 4.245                         | 4.249             |
| Maximum Acceleration: 911 g's |                   |