

Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.




Serial No: LW503298 Temperature: 23.8 °C
 Model: PIT ACC Humidity: 42%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
9.3 g's/volt
 R²: 0.999982 [Chip programmed]

Ref Acc 1: LW503313! Cal on: 31Jan2024
 10 g's/volt
 Ref Acc 2: LW503311! Cal on: 31Jan2024
 10 g's/volt

Operator: William Johnson




Signed

Calibration valid 2 years

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

From:
AUG 29 2024

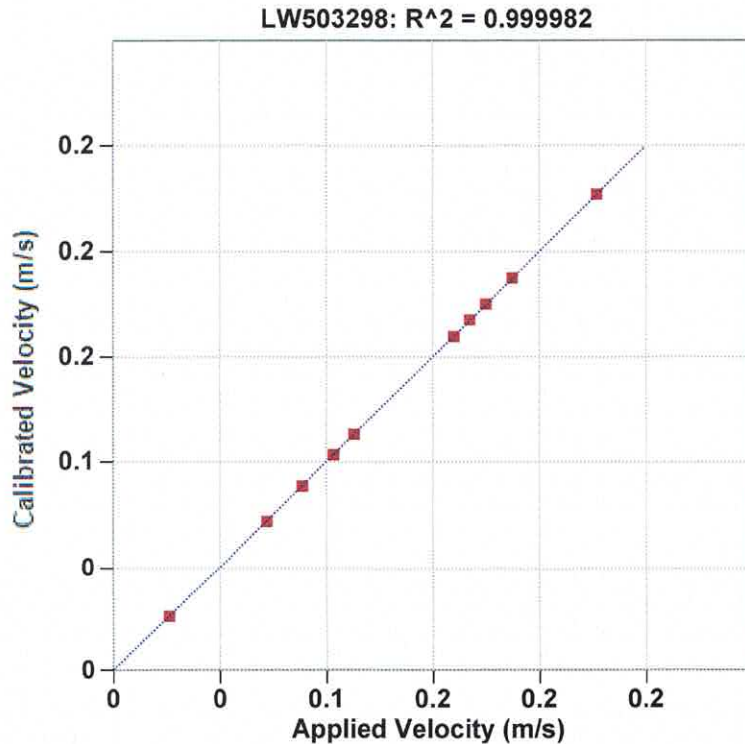

Reference Velocity	S/N LW503298 Velocity
m/s	m/s
0.026	0.026
0.072	0.072
0.089	0.089
0.104	0.103
0.113	0.113
0.160	0.160
0.167	0.168
0.175	0.175
0.187	0.188
0.227	0.227

Maximum Acceleration: 25 g's

