



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: T303


PDI Gage Factor: 146.4

Mean Linear Correlation Coefficient: 0.999675

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1981.6	-3.974	341.2	0.706
-1463.3	-2.962	761.2	1.517
-1076.1	-2.157	1168.0	2.277
-702.1	-1.401	1555.1	3.009
-387.1	-0.748	1935.7	3.726
-63.4	-0.089		

Calibration Curve

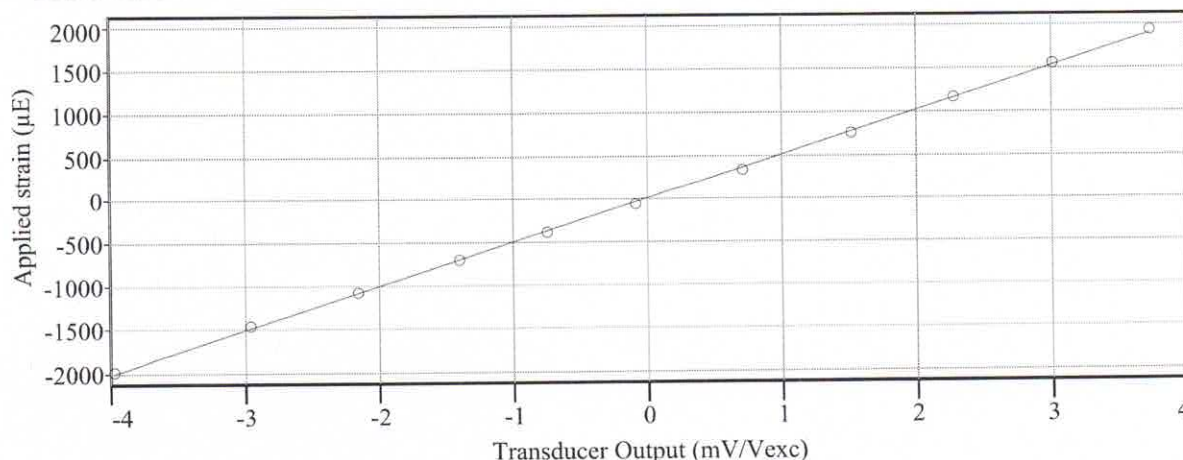

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: T303

Calibration Date: 8/22/2024 12:09:37 PM

