

Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer


Serial Number: X072

PDI Gage Factor: 91.5 Mean Linear Correlation Coefficient: 0.999961

Table 1: Representative Calibration Data

Applied strain (µE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2200.3	-6.844	365.3	1.293
-1679.8	-5.205	800.5	2.677
-1170.2	-3.603	1235.8	4.024
-721.8	-2.201	1640.4	5.273
-374.0	-1.083	1986.0	6.336
-32.8	0.016		

Calibration Curve

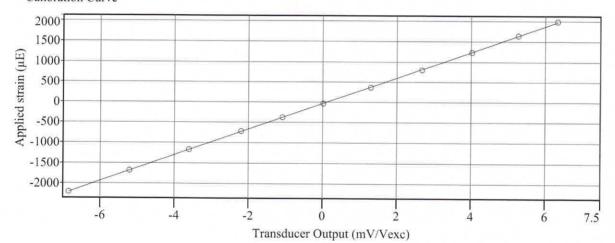

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: VANNA OUK

Signature:

PDI Gage: X072

Calibration Date:

