
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 197A
PDI Gage Factor: 92.3
Mean Linear Correlation Coefficient: 0.999981

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2001.3	-6.116	465.9	1.617
-1489.5	-4.521	866.1	2.873
-1003.9	-3.024	1187.7	3.870
-570.9	-1.653	1489.5	4.812
-216.5	-0.559	1791.3	5.741
98.4	0.435	2014.4	6.408

Calibration Curve

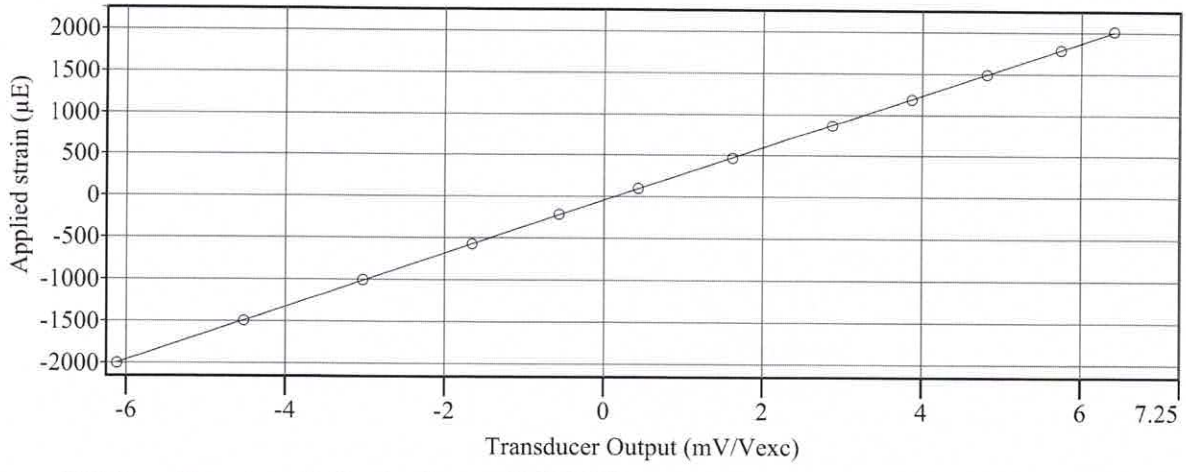

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: 197A

Calibration Date: SEP 2 5 2024

Pile Dynamics, Inc.