Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 246A
PDI Gage Factor: 93.9
Mean Linear Correlation Coefficient: 0.999972

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1929.1	-5.774	590.6	1.967
-1410.8	-4.173	990.8	3.234
-912.1	-2.653	1318.9	4.258
-459.3	-1.254	1653.5	5.251
-105.0	-0.183	1994.8	6.260
223.1	0.838		

Calibration Curve

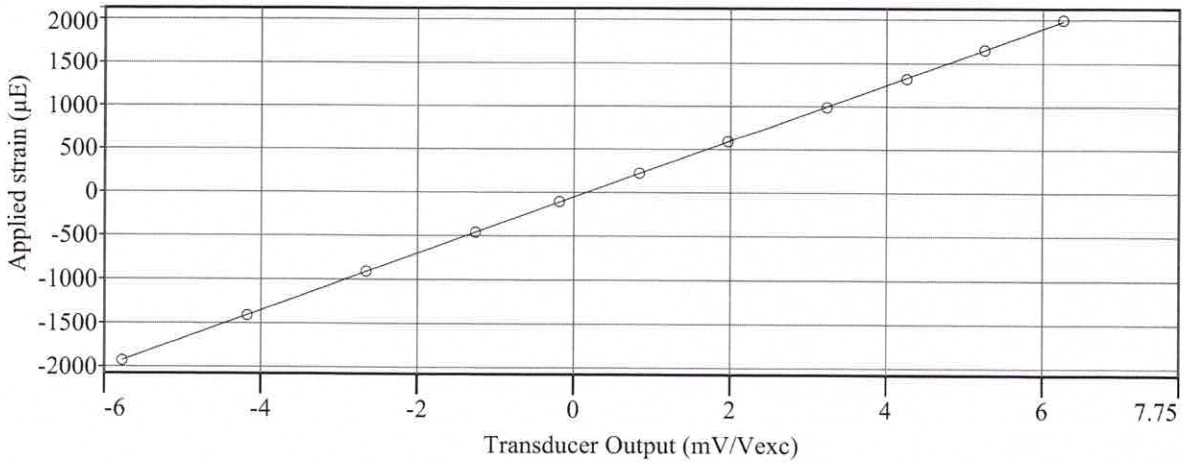

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kay Tol

Signature: Kay Tol

PDI Gage: 246A

Calibration Date: OCT 1 6 2024