

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 80473 Temperature: 23.0 °C
Model: PE Humidity: 42%
Calibrated on: Channel 3 on 8G 5161 LE


PDA CALIBRATION FACTOR

933.2 g's/volt

R²: 0.999967 [Chip programmed]


Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt

Operator: William Johnson


Signed

Calibration valid 2 years

From: ~~OCT 10 2024~~

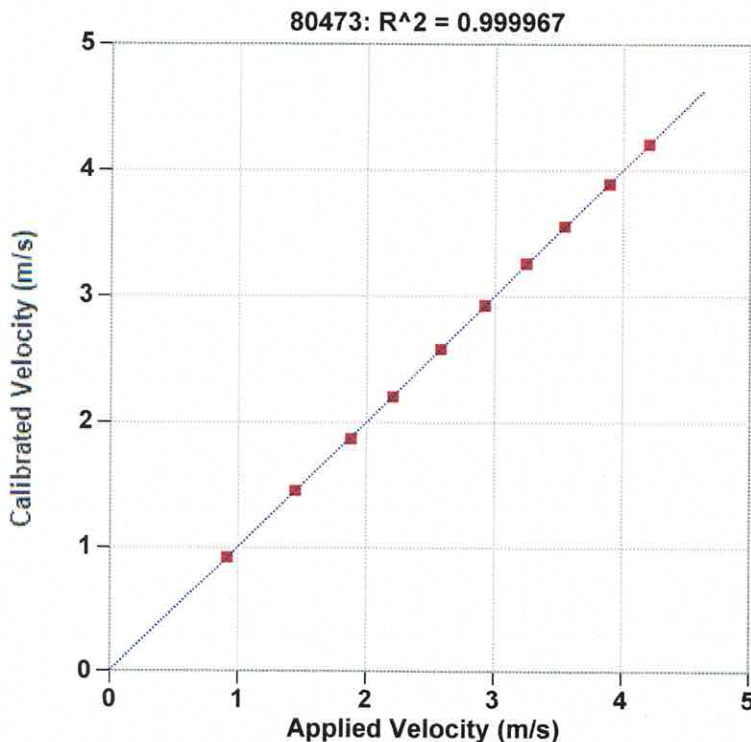

Reference Velocity	S/N 80473 Velocity
m/s	m/s
0.920	0.922
1.450	1.453
1.883	1.869
2.212	2.207
2.582	2.582
2.926	2.929
3.254	3.260
3.549	3.556
3.899	3.895
4.211	4.210

Maximum Acceleration: 918 g's

