
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 94A
PDI Gage Factor: 93.1
Mean Linear Correlation Coefficient: 0.999922

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2086.6	-6.434	393.7	1.343
-1594.5	-4.897	807.1	2.619
-1128.6	-3.424	1154.9	3.697
-669.3	-2.007	1469.8	4.643
-315.0	-0.887	1771.7	5.557
0.0	0.086	2021.0	6.261

Calibration Curve

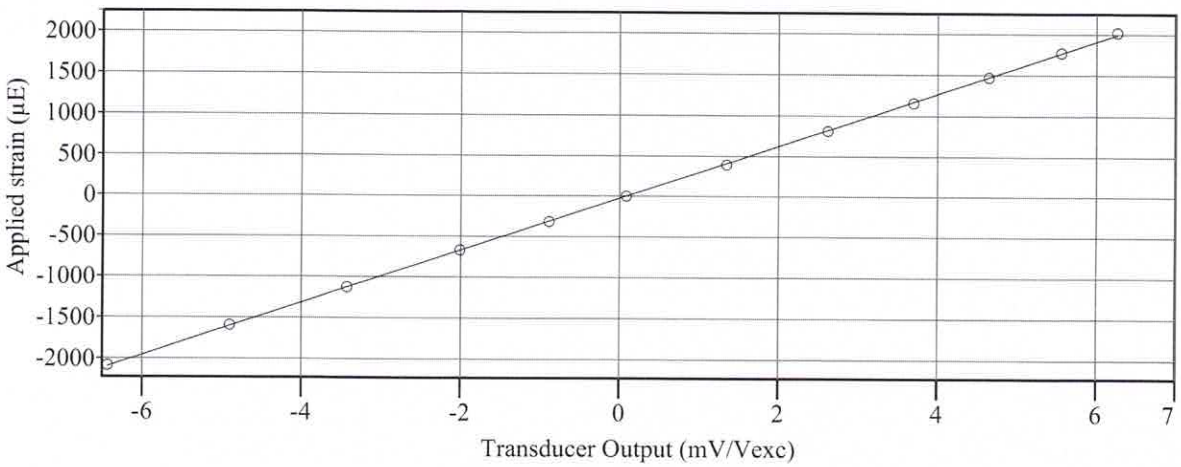

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: 94A

Calibration Date: SEP 2 5 2024