

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K11295 Temperature: 24.0 °C
Model: KICHER PR Humidity: 55%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

373.8 mv/5000g
(74.8 μv/g)
R^2: 0.999949 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 10Sep2024

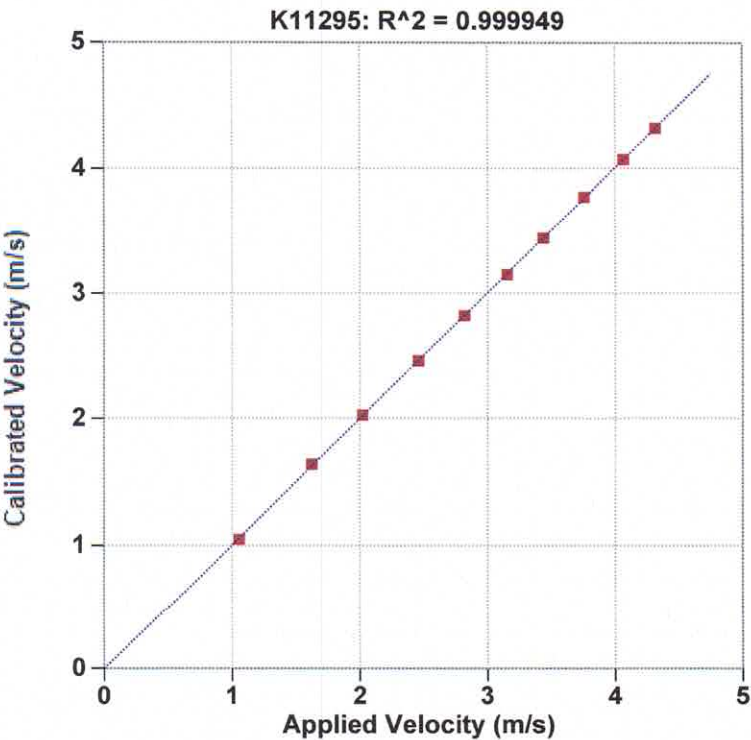

Reference Velocity	S/N K11295 Velocity
m/s	m/s
1.059	1.050
1.627	1.639
2.025	2.028
2.465	2.459
2.826	2.822
3.160	3.151
3.444	3.442
3.763	3.774
4.069	4.072
4.320	4.317

Maximum Acceleration: 941 g's