
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: K126
PDI Gage Factor: 90.7
Mean Linear Correlation Coefficient: 0.999709

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2132.5	-6.494	262.5	1.291
-1594.5	-4.766	638.7	2.461
-1122.0	-3.247	1010.5	3.613
-741.5	-2.008	1404.2	4.833
-439.6	-0.952	1778.2	5.973
-102.8	0.134	2021.0	6.671

Calibration Curve

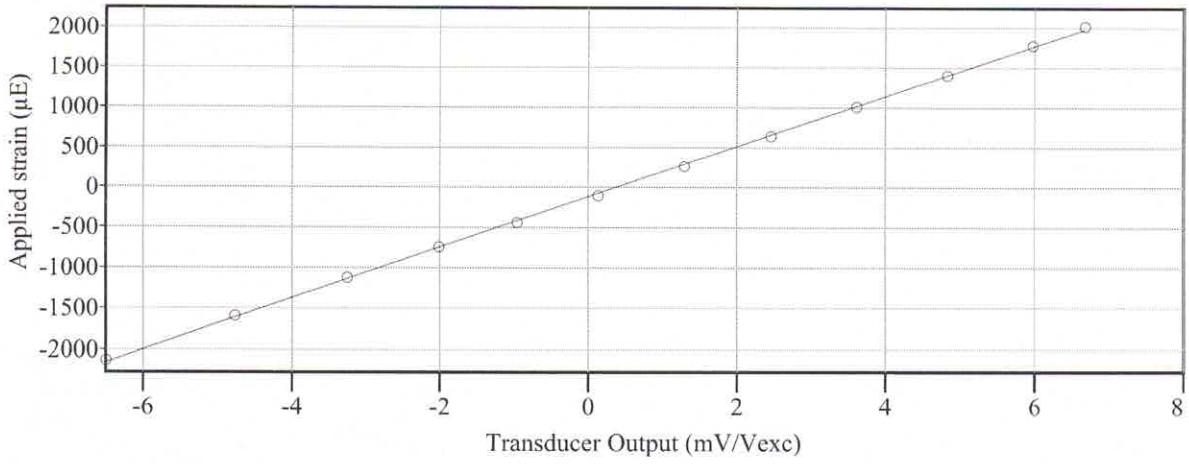

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: K126
Calibration Date: 9/17/24

Pile Dynamics, Inc.